

Calibration Data

Airtech Environmental Services, Inc. Meter Box Full Test Calibration

Date: 5/23/2011

Operator: iburton

Time	Meter Box ID M-3		Meter Box ΔH@		1.807		Meter Box Y _d		0.9891		Barometric Pressure (in. Hg.)		29.50			
	Orifice Data						Meter Box Data						Results			
θ (min)	K'	Vacuum	T _{amb}	V _{cr}	V _{initial}	V _{final}	V _d	ΔH	T _i	T _o	T _{avg}	V _{inlet}	V _{mid}	Q	Y _d	ΔH@
5.0	0.3445	20.0	76	2.195	740.70	742.98	2.28	0.64	75	73	74	742.98	2.225	0.439	0.9863	1.817
5.0	0.3445	20.0	76	2.195	742.98	745.27	2.29	0.64	76	74	75.0	745.27	2.231	0.439	0.9838	1.804
5.0	0.3445	20.0	76	2.195	745.27	747.57	2.30	0.64	76	74	75.0	747.57	2.241	0.439	0.9795	1.789
5.0	0.4436	19.0	76	2.826	748.00	750.96	2.96	1.10	77	74	75.5	750.96	2.884	0.565	0.9798	1.858
5.0	0.4436	19.0	76	2.826	750.96	753.90	2.94	1.10	78	75	76.5	753.90	2.859	0.565	0.9884	1.887
5.0	0.4436	19.0	76	2.826	753.90	756.85	2.95	1.10	79	75	77.0	756.85	2.867	0.565	0.9859	1.876
5.0	0.5885	17.0	77	3.746	757.20	761.09	3.89	1.8	81	76	78.5	761.09	3.776	0.749	0.9920	1.770
5.0	0.5885	17.0	77	3.746	761.09	764.99	3.90	1.8	82	76	79.0	764.99	3.782	0.749	0.9904	1.763
5.0	0.5885	17.0	77	3.746	764.99	768.89	3.90	1.8	83	77	80.0	768.89	3.775	0.749	0.9922	1.766
5.0	0.7954	15.0	77	5.063	769.50	774.76	5.26	3.3	86	78	82.0	769.50	5.092	1.013	0.9943	1.786
5.0	0.7954	15.0	77	5.063	774.76	780.04	5.28	3.3	88	79	83.5	780.04	5.097	1.013	0.9933	1.778
5.0	0.7954	15.0	77	5.063	780.04	785.32	5.28	3.3	98	80	89.0	785.32	5.046	1.013	1.0033	1.796
Average														0.9891	1.807	

Nomenclature	
K'	Critical Orifice Coefficient
T _{amb}	Ambient Temperature (°F)
V _{cr}	Volume Through Orifice (scf)
V _d	Gas Meter Volume (ft³)
ΔH	Orifice Pressure Differential (in. H ₂ O)
T _i	Meter Inlet Temperature (°F)
T _o	Meter Outlet Temperature (°F)
T _{avg}	Average Meter Box Temperature (°F)
V _{inlet}	Volume Metered Standardized (scf)
Q	Flow Rate (scfm)
Y _d	Meter Correction Factor (dimensionless)
ΔH@	ΔH yielding 0.75 scfm

Vacuum Gauge (in. Hg.)		Thermometers (°F)	
Standard	Volume Range	Or No	Ch No
5	5.0	1	2
10	10.0	33	33
15	15.0	51	51
20	20.0	101	101
25	25.0	152	151
		213	213
		252	252
		301	301
		352	352
		401	402
		502	502
		602	602

$$V_{cr} = K' \cdot P_b \cdot \theta \cdot (T_{amb} + 460)^{-0.5}$$

$$V_{mid} = 17.64 \cdot Y_d \cdot (P_b + \Delta H / 13.6) \cdot (T_o + 460)$$

$$Q = V_{cr} \cdot \theta$$

$$Y_d = V_{cr} / V_{mid}$$

$$\Delta H(@) = 0.319 \cdot \Delta H \cdot (T_{amb} + 460) \cdot \theta^2 \cdot P_b \cdot Y_d^2 \cdot V_m^2$$

Airtech Environmental Services Meter Post Calibration

Average Field Sample Rate (ΔH)	1.500	Date	7/27/2011
Highest Field Vacuum (inches Hg)	5	Client	BREC
Critical Orifice ID	AA-63	Project No.	3648
Orifice Flow Rate (cfm)	0.784	Meter ID	M-3

	Run 1	Run 2	Run 3
Initial Volume (ft ³)	248.00	251.92	255.84
Final Volume (ft ³)	251.92	255.84	259.75
Volume Metered (ft ³)	3.92	3.92	3.91
DGM Inlet Temperature (°F)	87	88	89
DGM Outlet Temperature (°F)	82	83	83
Average DGM Temperature (°F)	84.5	85.5	86.0
Ambient Temperature (°F)	80	80	80
Elapsed Time (min.)	5	5	5
ΔH (inches H ₂ O)	1.80	1.80	1.80
Barometric Pressure (inches Hg)	29.5	29.5	29.5
Pump Vacuum (inches Hg)	18	18	18
K'	0.5885	0.5885	0.5885
V _{cr} (ft ³)	3.735	3.735	3.735
V _{mstd} (ft ³)	3.763	3.756	3.743
Post Test Y _c	0.9926	0.9945	0.9979
Full Test Y _d	0.9891	0.9891	0.9891
% Difference	-0.36	-0.54	-0.89
Average % Difference			-0.60

Airtech Environmental Services, Inc.
Meter Box Full Test Calibration

Date: 4/13/2011

Operator: Lburton

Meter Box ID M-5										Meter Box $\Delta H @$			Meter Box Y_d			Barometric Pressure (in. Hg.)			Remarks	
Time	Office Data										Meter Box Data									
θ (min)	K'	Vacuum	T_{amb}	V_{er}	V_{inlet}	V_{final}	V_d	ΔH	T_i	T_o	T_{avg}	V_{mid}	Q	Y_c	$\Delta H @$					
5.0	0.3445	22.0	68	2.211	309.00	311.19	2.19	0.66	69	66	67.5	2.164	0.442	1.0219	1.995					
5.0	0.3445	22.0	66	2.216	311.19	313.38	2.19	0.66	71	67	69.0	2.158	0.443	1.0268	2.001					
5.0	0.3445	22.0	66	2.216	313.38	315.58	2.20	0.66	72	68	70.0	2.164	0.443	1.0240	1.986					
5.0	0.4436	21.0	66	2.853	315.90	318.83	2.93	1.10	73	69	71.0	2.879	0.571	0.9908	1.870					
5.0	0.4436	21.0	67	2.850	318.83	321.75	2.92	1.10	75	69	72.0	2.864	0.570	0.9952	1.886					
5.0	0.4436	21.0	67	2.850	321.75	324.69	2.94	1.10	76	70	73.0	2.878	0.570	0.9903	1.864					
5.0	0.5885	19.0	66	3.785	325.00	328.97	3.97	2.0	78	71	74.5	3.884	0.757	0.9744	1.864					
5.0	0.5885	19.0	66	3.785	328.97	332.93	3.96	2.0	80	72	76.0	3.864	0.757	0.9796	1.879					
5.0	0.5885	19.0	66	3.785	332.93	336.89	3.96	2.0	82	73	77.5	3.853	0.757	0.9823	1.884					
5.0	0.7954	17.0	66	5.115	337.30	342.73	5.43	3.7	86	74	80.0	5.281	1.023	0.9687	1.862					
5.0	0.7954	17.0	66	5.115	342.73	348.15	5.42	3.7	88	75	81.5	5.257	1.023	0.9731	1.874					
5.0	0.7954	17.0	66	5.115	348.15	353.58	5.43	3.7	91	76	83.5	5.247	1.023	0.9749	1.874					
													Average	0.9918	1.903					

Nomenclature	
K'	Critical Orifice Coefficient
T_{amb}	Ambient Temperature (°F)
V_{er}	Volume Through Orifice (scf)
V_d	Gas Meter Volume (ft³)
ΔH	Orifice Pressure Differential (in. H₂O)
T_i	Meter Inlet Temperature (°F)
T_o	Meter Outlet Temperature (°F)
T_{avg}	Average Meter Box Temperature (°F)
V_{mid}	Volume Metered Standardized (scf)
Q	Flow Rate (scfm)
Y_d	Meter Correction Factor (dimensionless)
$\Delta H @$	ΔH yielding 0.75 scfm

Vapour States (in. Hg.)			Thermodynamic (°F)					
Standard	Vapour	Grube	Size/Inch	Gr. No.	Gr. No.	Gr. No.	Gr. No.	
5	5.0	32	31	2	2	3	3	
10	10.0	50	49	51	32	31	31	
15	15.0	100	99	101	51	50	50	
20	20.0	150	149	151	101	100	100	
25	25.0	212	213	213	151	150	150	
		250	251	251	213	212	212	
		300	301	301	251	251	251	
		350	351	351	301	301	301	
		400	400	402	351	350	350	
		500	500	502	402	400	400	
		600	601	602	502	501	501	

$V_c = K' * P_b * \theta$
 $(T_{amb} + 460)^{0.5}$
 $V_{mid} = 17.64 * Y_d * (P_b + \Delta H / 13.6)$
 $(T_{avg} + 460)$
 $Q = V_{er} * \theta$
 $Y_d = V_{er} / V_{mid}$
 $\Delta H @ = .0319 * \Delta H * (T_{avg} + 460) * \theta^2$
 $P_b * Y_d^2 * V_d^2$

Airtech Environmental Services Meter Post Calibration

Average Field Sample Rate (ΔH)	2.000	Date	7/27/2011
Highest Field Vacuum (inches Hg)	11	Client	BREC
Critical Orifice ID	AA-63	Project No.	3648
Orifice Flow Rate (cfm)	0.778	Meter ID	M-5

	Run 1	Run 2	Run 3
Initial Volume (ft ³)	702.00	705.89	709.79
Final Volume (ft ³)	705.89	709.79	713.69
Volume Metered (ft ³)	3.89	3.90	3.90
DGM Inlet Temperature (°F)	81	83	88
DGM Outlet Temperature (°F)	77	78	81
Average DGM Temperature (°F)	79.0	80.5	84.5
Ambient Temperature (°F)	80	79	79
Elapsed Time (min.)	5	5	5
ΔH (inches H ₂ O)	2.00	2.00	2.00
Barometric Pressure (inches Hg)	29.5	29.5	29.5
Pump Vacuum (inches Hg)	20	20	20
K'	0.5885	0.5885	0.5885
Ver (ft ³)	3.735	3.739	3.739
Vmstd (ft ³)	3.774	3.774	3.746
Post Test Yc	0.9897	0.9908	0.9982
Full Test Yd	0.9953	0.9953	0.9953
% Difference	0.56	0.45	-0.29
Average % Difference			0.24

Airtech Environmental Services, Inc.
Meter Box Full Test Calibration

Date: 9/13/2010

Operator: Iburton

Time	Orifice Data					Meter Box ΔH@					Meter Box Y _d					Barometric Pressure (in. Hg.)					Results				
	θ (min)	K'	Vacuum	T _{amb}	V _{or}	V _{initial}	V _{final}	V _d	ΔH	T _i	T _o	T _{avg}	V _{maid}	Q	Y _d	ΔH@									
5.0	0.3455	22.0	85	2.183	466.60	468.84	2.24	0.61	84	82	83	2.150	0.437	1.0153	1.758										
5.0	0.3455	22.0	86	2.181	468.84	471.09	2.25	0.61	84	82	83.0	2.160	0.436	1.0099	1.742										
5.0	0.3455	22.0	86	2.181	471.09	473.34	2.25	0.61	85	83	84.0	2.156	0.436	1.0118	1.746										
5.0	0.4434	21.0	86	2.799	475.40	478.33	2.93	1.05	86	84	85.0	2.805	0.560	0.9978	1.775										
5.0	0.4434	21.0	88	2.794	478.33	481.22	2.89	1.05	86	84	85.0	2.767	0.559	1.0098	1.825										
5.0	0.4434	21.0	88	2.794	481.22	484.12	2.90	1.05	87	85	86.0	2.771	0.559	1.0082	1.815										
5.0	0.5926	19.0	88	3.734	484.50	488.39	3.89	1.9	87	85	86.0	3.725	0.747	1.0024	1.826										
5.0	0.5926	19.0	89	3.731	488.39	492.28	3.89	1.9	87	86	86.5	3.722	0.746	1.0024	1.827										
5.0	0.5926	19.0	89	3.731	492.28	496.17	3.89	1.9	87	86	86.5	3.722	0.746	1.0024	1.827										
5.0	0.7965	17.0	90	5.010	496.80	501.97	5.17	3.25	88	86	87.0	4.958	1.002	1.0103	1.771										
5.0	0.7965	17.0	90	5.010	501.97	507.15	5.18	3.25	89	87	88.0	4.959	1.002	1.0102	1.768										
5.0	0.7965	17.0	90	5.010	507.15	512.33	5.18	3.25	89	87	88.0	4.959	1.002	1.0102	1.768										
														Average	1.0076	1.787									

Vacuum Scale (in. Hg.)	Temperature (°F)	Summary					
		CP. NO.	CR. NO.	CR. NO.	CR. NO.	CR. NO.	CR. NO.
5	5.0	32	31	2	3		
10	10.0	50	49	50			
15	15.0	100	98	99			
20	20.0	150	148	159			
25	25.0	212	209	212			
		250	247	250			
		300	297	299			
		350	347	349			
		400	396	400			
		500	497	500			
		600	601	598			

$$V_{cr} = K' * P_b * \theta$$

$$(T_{amb} + 460) \wedge 0.5$$

$$V_{maid} = 17.64 * Y_d * (P_b + \Delta H / 13.6)$$

$$(T_{avg} + 460)$$

$$Q = V_{cr} / \theta$$

$$Y_d = V_{cr} / V_{maid}$$

$$\Delta H(@) = .0319 * \Delta H * (T_{amb} + 460) * \rho * C^2$$

$$P_b * Y_d^2 * V_{cr}^2$$

Nomenclature	
K'	Critical Orifice Coefficient
T _{amb}	Ambient Temperature (°F)
V _{or}	Volume Through Orifice (scf)
V _d	Gas Meter Volume (ft³)
ΔH	Orifice Pressure Differential (in. H ₂ O)
T _i	Meter Inlet Temperature (°F)
T _o	Meter Outlet Temperature (°F)
T _{avg}	Average Meter Box Temperature (°F)
V _{maid}	Volume Metered Standardized (scf)
Q	Flow Rate (scfm)
Y _d	Meter Correction Factor (dimensionless)
ΔH@	ΔH yielding 0.75 scfm

Airtech Environmental Services Meter Post Calibration

Average Field Sample Rate (ΔH)	1.500	Date	8/2/2011
Highest Field Vacuum (inches Hg)	10	Client	BREC
Critical Orifice ID	AA-63	Project No.	3648
Orifice Flow Rate (cfm)	0.766	Meter ID	M-6

	Run 1	Run 2	Run 3
Initial Volume (ft ³)	69.00	72.83	76.64
Final Volume (ft ³)	72.83	76.64	80.47
Volume Metered (ft ³)	3.83	3.81	3.83
DGM Inlet Temperature (°F)	90	91	92
DGM Outlet Temperature (°F)	87	88	89
Average DGM Temperature (°F)	88.5	89.5	90.5
Ambient Temperature (°F)	90	90	91
Elapsed Time (min.)	5	5	5
ΔH (inches H ₂ O)	1.80	1.80	1.80
Barometric Pressure (inches Hg)	29.5	29.5	29.5
Pump Vacuum (inches Hg)	19	19	19
K'	0.5885	0.5885	0.5885
V _{cr} (ft ³)	3.701	3.701	3.698
V _{mstd} (ft ³)	3.650	3.624	3.637
Post Test Yc	1.0141	1.0213	1.0168
Full Test Yd	1.0076	1.0076	1.0076
% Difference	-0.64	-1.36	-0.92
Average % Difference			-0.97

Airtech Environmental Services, Inc.
Meter Box Full Test Calibration

Date: 2/1/2011 Operator: jburton

Time	Orifice Data								Meter Box Data										Repeats
	K'	Vacuum	T _{amb}	V _{cr}	V _{initial}	V _{final}	V _d	ΔH	T _i	T _o	T _{avg}	V _{maid}	Q	Y _d	ΔH@				
5.0	0.3455	22.0	64	2.226	310.10	312.38	2.28	0.66	67	65	66	2.259	0.445	0.9854	1.845				
5.0	0.3455	22.0	65	2.224	312.38	314.65	2.27	0.66	68	67	67.5	2.243	0.445	0.9916	1.867				
5.0	0.3455	22.0	66	2.222	314.65	316.92	2.27	0.66	68	67	67.5	2.243	0.444	0.9906	1.867				
5.0	0.4434	21.0	66	2.852	317.20	320.13	2.93	1.10	69	67	68.0	2.896	0.570	0.9848	1.869				
5.0	0.4434	21.0	66	2.852	320.13	323.07	2.94	1.10	70	68	69.0	2.900	0.570	0.9833	1.860				
5.0	0.4434	21.0	66	2.852	323.07	325.99	2.92	1.10	71	68	69.5	2.878	0.570	0.9910	1.888				
5.0	0.5926	19.0	66	3.811	326.20	330.11	3.91	1.9	72	68	70.0	3.857	0.762	0.9881	1.820				
5.0	0.5926	19.0	67	3.808	330.11	334.02	3.91	1.9	72	69	70.5	3.854	0.762	0.9881	1.822				
5.0	0.5926	19.0	67	3.808	334.02	337.93	3.91	1.9	74	70	72.0	3.843	0.762	0.9909	1.827				
5.0	0.7965	17.0	66	5.123	338.30	343.56	5.26	3.5	77	71	74.0	5.171	1.025	0.9907	1.867				
5.0	0.7965	17.0	66	5.123	343.56	348.82	5.26	3.5	79	71	75.0	5.161	1.025	0.9926	1.870				
5.0	0.7965	17.0	66	5.123	348.82	354.09	5.27	3.5	80	72	76.0	5.161	1.025	0.9925	1.866				
													Average	0.9891	1.856				

Nomenclature		Temperature (°F)						Equations	
K'	Critical Orifice Coefficient	Orifice Inlet Temp (°F)						Equations	
T _{amb}	Ambient Temperature (°F)	Orifice Inlet Temp (°F)	Orifice Inlet Temp (°F)	Orifice Inlet Temp (°F)	Orifice Inlet Temp (°F)	Orifice Inlet Temp (°F)	Orifice Inlet Temp (°F)	Orifice Inlet Temp (°F)	Orifice Inlet Temp (°F)
V _{cr}	Volume Through Orifice (scf)	5	10	15	20	25	30	35	40
V _d	Gas Meter Volume (ft ³)	31	49	99	150	212	251	301	351
ΔH	Orifice Pressure Differential (in. H ₂ O)	32	50	100	150	212	251	301	351
T _i	Meter Inlet Temperature (°F)	31	49	99	150	212	251	301	351
T _o	Meter Outlet Temperature (°F)	50	99	150	212	251	301	351	401
T _{avg}	Average Meter Box Temperature (°F)	66	75	80	85	90	95	100	105
V _{maid}	Volume Metered Standardized (scf)	32	49	100	150	212	251	301	351
Q	Flow Rate (scfm)	32	49	100	150	212	251	301	351
Y _d	Meter Correction Factor (dimensionless)	32	49	100	150	212	251	301	351
ΔH@	ΔH yielding 0.75 scfm	32	49	100	150	212	251	301	351

$$V_{cr} = K' \cdot P_o \cdot \theta$$

$$\theta = \sqrt{(T_{amb} + 460) \cdot 0.5}$$

$$V_{maid} = 17.64 \cdot V_d \cdot \left(\frac{P_o}{(T_{avg} + 460)} \right)$$

$$Q = V_{cr} / \theta$$

$$Y_d = V_{cr} / V_{maid}$$

$$\Delta H@ = .0219 \cdot \Delta H \cdot (T_{amb} + 460) \cdot \theta^2$$

$$P_o \cdot Y_d^2 = V_{maid}^2$$

Airtech Environmental Services Meter Post Calibration

Average Field Sample Rate (ΔH)	1.300	Date	7/27/2011
Highest Field Vacuum (inches Hg)	10	Client	BREC
Critical Orifice ID	AA-63	Project No.	3648
Orifice Flow Rate (cfm)	0.778	Meter ID	M-9

	Run 1	Run 2	Run 3
Initial Volume (ft ³)	244.50	248.39	252.29
Final Volume (ft ³)	248.39	252.29	256.19
Volume Metered (ft ³)	3.89	3.90	3.90
DGM Inlet Temperature (°F)	82	84	84
DGM Outlet Temperature (°F)	79	80	80
Average DGM Temperature (°F)	80.5	82.0	82.0
Ambient Temperature (°F)	84	83	84
Elapsed Time (min.)	5	5	5
ΔH (inches H ₂ O)	1.90	1.90	1.90
Barometric Pressure (inches Hg)	29.5	29.5	29.5
Pump Vacuum (inches Hg)	20	20	20
K'	0.5885	0.5885	0.5885
V _{cr} (ft ³)	3.722	3.725	3.722
V _{mstd} (ft ³)	3.763	3.762	3.762
Post Test Y _c	0.9890	0.9901	0.9892
Full Test Y _d	0.9891	0.9891	0.9891
% Difference	0.01	-0.11	-0.01
Average % Difference			-0.04

Airtech Environmental Services Meter Post Calibration

Average Field Sample Rate (ΔH)	1.300	Date	7/27/2011
Highest Field Vacuum (inches Hg)	10	Client	BREC
Critical Orifice ID	AA-63	Project No.	3648
Orifice Flow Rate (cfm)	0.762	Meter ID	M-10

	Run 1	Run 2	Run 3
Initial Volume (ft ³)	884.60	888.41	892.23
Final Volume (ft ³)	888.41	892.23	896.04
Volume Metered (ft ³)	3.81	3.82	3.81
DGM Inlet Temperature (°F)	83	84	85
DGM Outlet Temperature (°F)	81	81	81
Average DGM Temperature (°F)	82.0	82.5	83.0
Ambient Temperature (°F)	88	88	89
Elapsed Time (min.)	5	5	5
ΔH (inches H ₂ O)	1.80	1.80	1.80
Barometric Pressure (inches Hg)	29.5	29.5	29.5
Pump Vacuum (inches Hg)	17	17	17
K'	0.5885	0.5885	0.5885
V _{cr} (ft ³)	3.708	3.708	3.705
V _{mstd} (ft ³)	3.674	3.681	3.668
Post Test Y _c	1.0092	1.0074	1.0101
Full Test Y _d	1.0091	1.0091	1.0091
% Difference	-0.01	0.16	-0.10
Average % Difference			0.02

Airtech Environmental Services, Inc.
Meter Box Full Test Calibration

Date: 9/13/2010
Operator: jburton

Meter Box ID M-14		Orifice Data				Meter Box Yd				Barometric Pressure (in. Hg.)				Results			
Time	θ (min)	K'	Vacuum	T _{amb}	V _{cr}	V _{initial}	V _{final}	V _d	ΔH	T ₁	T ₂	T _{avg}	V _{meas}	Q	Y _d	ΔH@	
5.0		0.3455	22.0	83	2.187	510.30	512.57	2.27	0.63	82	89	85.5	2.169	0.437	1.0083	1.772	
5.0		0.3455	22.0	83	2.187	512.57	514.83	2.26	0.63	83	80	81.5	2.175	0.437	1.0054	1.775	
5.0		0.3455	22.0	83	2.187	514.83	517.09	2.26	0.63	84	81	82.5	2.171	0.437	1.0072	1.778	
5.0		0.4434	20.0	84	2.804	517.40	520.33	2.93	1.05	85	82	83.5	2.813	0.561	0.9969	1.766	
5.0		0.4434	20.0	84	2.804	523.27	523.27	2.94	1.05	87	82	84.5	2.817	0.561	0.9954	1.757	
5.0		0.4434	20.0	84	2.804	526.17	526.17	2.90	1.05	89	83	86.0	2.771	0.561	1.0119	1.811	
5.0		0.5926	18.0	84	3.748	526.60	530.50	3.90	1.9	91	84	87.5	3.724	0.750	1.0062	1.817	
5.0		0.5926	18.0	84	3.748	530.50	534.40	3.90	1.9	93	85	89.0	3.714	0.750	1.0090	1.822	
5.0		0.5926	18.0	84	3.748	534.40	538.30	3.90	1.9	94	86	90.0	3.707	0.750	1.0108	1.826	
5.0		0.7965	15.0	84	5.037	538.90	544.13	5.23	3.4	97	87	92.0	4.972	1.007	1.0130	1.823	
5.0		0.7965	15.0	84	5.037	544.13	549.36	5.23	3.4	100	89	94.5	4.950	1.007	1.0176	1.831	
5.0		0.7965	15.0	84	5.037	549.36	554.58	5.22	3.4	102	90	96.0	4.927	1.007	1.0223	1.843	
															Average	1.0087	1.802

Nomenclature	
K'	Critical Orifice Coefficient
T _{amb}	Ambient Temperature (°F)
V _{cr}	Volume Through Orifice (scf)
V _d	Gas Meter Volume (ft³)
ΔH	Orifice Pressure Differential (in. H₂O)
T ₁	Meter Inlet Temperature (°F)
T ₂	Meter Outlet Temperature (°F)
T _{avg}	Average Meter Box Temperature (°F)
V _{meas}	Volume Metered Standardized (scf)
Q	Flow Rate (scfm)
Y _d	Meter Correction Factor (dimensionless)
ΔH@	ΔH yielding 0.75 scfm

Vacuum Gauges (in. Hg.)		Thermometers (°F)			
Standard	Vacuum Gauge	GA No.	CR No.	CR No.	CR No.
5	5.0	32	32	33	32
10	10.0	50	51	51	50
15	15.0	100	100	101	100
20	20.0	150	151	151	150
25	25.0	212	213	213	212
		250	251	251	250
		300	300	301	300
		350	350	350	349
		400	400	400	399
		500	500	500	498
		600	600	599	598

$$V_{cr} = K' * P_b * \theta / (T_{amb} + 460) ^ 0.5$$

$$V_{meas} = 17.64 * V_d * (P_b + \Delta H / 13.6) / (T_{avg} + 460)$$

$$Q = V_{cr} / \theta$$

$$Y_d = V_{cr} / V_{meas}$$

$$\Delta H@ = -0.319 * \Delta H * (\pi_{cr} + 460) * \theta ^ 2 / (P_b * Y_d ^ 2 * V_{cr} ^ 2)$$

Airtech Environmental Services Meter Post Calibration

Average Field Sample Rate (ΔH)	1.300	Date	7/27/2011
Highest Field Vacuum (inches Hg)	10	Client	BREC
Critical Orifice ID	AA-63	Project No.	3648
Orifice Flow Rate (cfm)	0.754	Meter ID	M-14

	Run 1	Run 2	Run 3
Initial Volume (ft ³)	603.10	606.87	610.63
Final Volume (ft ³)	606.87	610.63	614.40
Volume Metered (ft ³)	3.77	3.76	3.77
DGM Inlet Temperature (°F)	82	83	84
DGM Outlet Temperature (°F)	78	78	78
Average DGM Temperature (°F)	80.0	80.5	81.0
Ambient Temperature (°F)	86	87	88
Elapsed Time (min.)	5	5	5
ΔH (inches H ₂ O)	1.80	1.80	1.80
Barometric Pressure (inches Hg)	29.5	29.5	29.5
Pump Vacuum (inches Hg)	18	18	18
K'	0.5885	0.5885	0.5885
V _{cr} (ft ³)	3.715	3.711	3.708
V _{mstd} (ft ³)	3.649	3.636	3.643
Post Test Y _c	1.0180	1.0207	1.0180
Full Test Y _d	1.0087	1.0087	1.0087
% Difference	-0.92	-1.19	-0.92
Average % Difference			-1.01

Airtech Environmental Services, Inc.
Meter Box Full Test Calibration

Date: 2/3/2011

Operator: i.burton

Time	Orifice Data						Meter Box ΔH @				Meter Box Y_d				Barometric Pressure (in. Hg.)				Remarks
	K'	Vacuum	T_{amb}	V_{or}	V_{final}	V_d	ΔH	T_i	T_o	T_{avg}	V_{inlet}	Q	Y_d	$\Delta H@$					
5.0	0.3455	22.0	76	2.201	23.00	25.19	2.19	68	69.5	2.156	0.440	1.0211	1.880						
5.0	0.3455	22.0	76	2.201	25.19	27.38	2.19	68	70.0	2.154	0.440	1.0220	1.882						
5.0	0.3455	22.0	76	2.201	27.38	29.56	2.18	69	71.0	2.140	0.440	1.0287	1.902						
5.0	0.4434	21.0	76	2.825	30.50	33.36	2.86	71	72.0	2.805	0.565	1.0070	1.874						
5.0	0.4434	21.0	76	2.825	33.36	36.22	2.86	72	73.0	2.800	0.565	1.0089	1.878						
5.0	0.4434	21.0	76	2.825	36.22	39.07	2.85	72	73.5	2.788	0.565	1.0134	1.893						
5.0	0.5926	19.0	76	3.775	39.60	43.43	3.83	73	75.0	3.743	0.755	1.0088	1.767						
5.0	0.5926	19.0	76	3.775	43.43	47.22	3.79	73	75.5	3.700	0.755	1.0204	1.807						
5.0	0.5926	19.0	76	3.775	47.22	51.05	3.83	74	77.0	3.729	0.755	1.0126	1.774						
5.0	0.7965	17.0	76	5.075	51.40	56.55	5.15	74	78.5	5.019	1.015	1.0111	1.808						
5.0	0.7965	17.0	76	5.075	56.55	61.68	5.13	75	79.5	4.990	1.015	1.0169	1.826						
5.0	0.7965	17.0	76	5.075	61.68	66.81	5.13	76	81.0	4.976	1.015	1.0197	1.831						
Average													1.0159	1.843					

Nomenclature	Value	Thermometers (°F)				Barometers (in. Hg.)				Equations		
		Orifice	Standard	Orifice	Standard	Orifice	Standard	Orifice	Standard	Equation	Result	
K'	Critical Orifice Coefficient											
T_{amb}	Ambient Temperature (°F)	1	31	2	32							
V_{or}	Volume Through Orifice (scf)		49		50							
V_d	Gas Meter Volume (ft³)		99		101							
ΔH	Orifice Pressure Differential (in. H ₂ O)		150		151							
T_i	Meter Inlet Temperature (°F)		212		213							
T_o	Meter Outlet Temperature (°F)		250		252							
T_{avg}	Average Meter Box Temperature (°F)		300		302							
V_{inlet}	Volume Metered Standardized (scf)		350		352							
Q	Flow Rate (scfm)		400		402							
Y_d	Meter Correction Factor (dimensionless)		500		502							
$\Delta H@$	ΔH yielding 0.75 scfm		600		602							

$$V_{or} = K' \cdot P_b \cdot \theta \cdot \left(\frac{P_b}{T_{mb} + 460} \right)^{0.5}$$

$$V_{inlet} = 17.64 \cdot V_d \cdot \left(\frac{P_b}{T_{avg} + 460} \right) \cdot (P_b + \Delta H / 13.6)$$

$$Q = V_{or} / \theta$$

$$Y_d = V_{or} / V_{inlet}$$

$$\Delta H@ = \frac{0.0319 \cdot \Delta H \cdot (T_{in} + 460) \cdot 9.2}{P_b \cdot Y_d^2 \cdot V_{or}^2}$$

Airtech Environmental Services Meter Post Calibration

Average Field Sample Rate (ΔH)	1.500	Date	8/9/2011
Highest Field Vacuum (inches Hg)	10	Client	BREC
Critical Orifice ID	AA-63	Project No.	3648
Orifice Flow Rate (cfm)	0.75	Meter ID	M-15

	Run 1	Run 2	Run 3
Initial Volume (ft ³)	174.50	178.25	182.02
Final Volume (ft ³)	178.25	182.02	185.78
Volume Metered (ft ³)	3.75	3.77	3.76
DGM Inlet Temperature (°F)	85	86	87
DGM Outlet Temperature (°F)	79	80	80
Average DGM Temperature (°F)	82.0	83.0	83.5
Ambient Temperature (°F)	85	85	85
Elapsed Time (min.)	5	5	5
ΔH (inches H ₂ O)	1.80	1.80	1.80
Barometric Pressure (inches Hg)	29.5	29.5	29.5
Pump Vacuum (inches Hg)	19	19	19
K'	0.5885	0.5885	0.5885
V _{cr} (ft ³)	3.718	3.718	3.718
V _{mstd} (ft ³)	3.617	3.629	3.616
Post Test Y _c	1.0281	1.0246	1.0282
Full Test Y _d	1.0159	1.0159	1.0159
% Difference	-1.20	-0.85	-1.21
Average % Difference			-1.09

Airtech Environmental Services Meter Post Calibration

Average Field Sample Rate (ΔH)	1.500	Date	8/9/2011
Highest Field Vacuum (inches Hg)	10	Client	BREC
Critical Orifice ID	AA-63	Project No.	3648
Orifice Flow Rate (cfm)	0.772	Meter ID	M-16

	Run 1	Run 2	Run 3
Initial Volume (ft³)	627.50	631.36	635.21
Final Volume (ft³)	631.36	635.21	639.08
Volume Metered (ft³)	3.86	3.85	3.87
DGM Inlet Temperature (°F)	86	87	88
DGM Outlet Temperature (°F)	82	82	82
Average DGM Temperature (°F)	84.0	84.5	85.0
Ambient Temperature (°F)	88	87	87
Elapsed Time (min.)	5	5	5
ΔH (inches H₂O)	1.80	1.80	1.80
Barometric Pressure (inches Hg)	29.5	29.5	29.5
Pump Vacuum (inches Hg)	20	20	20
K'	0.5885	0.5885	0.5885
V_{cr} (ft³)	3.708	3.711	3.711
V_{mstd} (ft³)	3.709	3.696	3.712
Post Test Y_c	0.9998	1.0042	0.9999
Full Test Y_d	0.9907	0.9907	0.9907
% Difference	-0.91	-1.36	-0.93
Average % Difference			-1.07

Airtech Environmental Services, Inc.
Meter Box Full Test Calibration

Date: 12/14/2010

Operator: Jburton

Meter Box ID M-17		Meter Box ΔH@				Meter Box Y _d				Meter Box ΔH@				Barometric Pressure (in. Hg.)				Results
Time		Orifice Data		Meter Box ΔH@		Meter Box Y _d		Meter Box ΔH@		Meter Box ΔH@		Meter Box ΔH@		Barometric Pressure (in. Hg.)		Results		
θ (min)	K'	Vacuum	T _{amb}	V _{cr}	V _{initial}	V _{final}	V _d	ΔH	T _i	T _o	T _{avg}	V _{meas}	Q	Y _d	ΔH@			
5.0	0.3455	22.0	76	2.201	780.30	782.52	2.22	0.63	72	68	70	2.163	0.440	1.0083	1.781			
5.0	0.3455	22.0	76	2.201	782.52	784.73	2.21	0.63	73	69	71.0	2.169	0.440	1.0147	1.801			
5.0	0.3455	22.0	76	2.201	784.73	786.94	2.21	0.63	73	69	71.0	2.169	0.440	1.0147	1.801			
5.0	0.4434	20.0	75	2.828	787.30	790.15	2.85	1.05	74	69	71.5	2.798	0.566	1.0107	1.806			
5.0	0.4434	20.0	75	2.828	790.15	793.01	2.86	1.05	74	70	72.0	2.805	0.566	1.0081	1.795			
5.0	0.4434	20.0	75	2.828	793.01	795.86	2.85	1.05	75	70	72.5	2.792	0.566	1.0126	1.810			
5.0	0.5926	18.0	76	3.775	796.20	800.01	3.81	1.8	76	70	73.0	3.736	0.755	1.0104	1.737			
5.0	0.5926	18.0	76	3.775	800.01	803.81	3.80	1.8	78	71	74.5	3.716	0.755	1.0159	1.751			
5.0	0.5926	18.0	76	3.775	803.81	807.63	3.82	1.8	79	71	75.0	3.732	0.755	1.0116	1.735			
5.0	0.7965	16.0	78	5.065	806.20	813.27	5.07	3.2	81	72	76.5	4.957	1.013	1.0218	1.756			
5.0	0.7965	16.0	78	5.065	813.27	818.37	5.10	3.2	83	73	78.0	4.972	1.013	1.0187	1.740			
5.0	0.7965	16.0	78	5.065	818.37	823.46	5.09	3.2	84	73	78.5	4.958	1.013	1.0216	1.748			
														Average	1.0141	1.772		

Notations		Thermometers (°F)					Equipments											
		1	2	3	4	5	6	7	8									
K'	Critical Orifice Coefficient																	
T _{amb}	Ambient Temperature (°F)																	
V _{cr}	Volume Through Orifice (scf)																	
V _d	Gas Meter Volume (ft ³)																	
ΔH	Orifice Pressure Differential (in. H ₂ O)																	
T _i	Meter Inlet Temperature (°F)																	
T _o	Meter Outlet Temperature (°F)																	
T _{avg}	Average Meter Box Temperature (°F)																	
V _{meas}	Volume Metered Standardized (scf)																	
Q	Flow Rate (scfm)																	
Y _d	Meter Correction Factor (dimensionless)																	
ΔH@	ΔH yielding 0.75 scfm																	

Vacuum Gauge (in. Hg.)		Thermometers (°F)			Equipments		
		1	2	3	4	5	6
5	5.0	32	33	33	33	33	
10	10.0	50	51	51	51	51	
15	15.0	100	101	101	102	102	
20	20.0	150	151	151	152	152	
25	25.0	212	213	213	214	214	
		250	251	251	252	252	
		300	301	301	303	303	
		350	352	352	353	353	
		400	401	401	402	403	
		500	501	501	503	503	
		600	601	601	602	603	

$$V_{cr} = K' \cdot P_a \cdot \theta$$

$$\sqrt{(T_{amb} + 460) \cdot 0.5}$$

$$V_{meas} = 17.64 \cdot V_d \cdot (P_a + 460) \cdot (\Delta H / 13.6)$$

$$Q = V_{cr} / \theta$$

$$Y_d = V_{cr} / V_{meas}$$

$$\Delta H@ = \frac{0.319 \cdot \Delta H \cdot (T_{avg} + 460) \cdot \rho \cdot 2}{P_a \cdot Y_c \cdot 2 \cdot V_m \cdot 2}$$

Airtech Environmental Services

Meter Post Calibration

Average Field Sample Rate (ΔH)	1.500	Date	8/8/2011
Highest Field Vacuum (inches Hg)	10	Client	BREC
Critical Orifice ID	AA-63	Project No.	3648
Orifice Flow Rate (cfm)	0.754	Meter ID	M-17

	Run 1	Run 2	Run 3
Initial Volume (ft ³)	267.50	271.27	275.05
Final Volume (ft ³)	271.27	275.05	278.81
Volume Metered (ft ³)	3.77	3.78	3.76
DGM Inlet Temperature (°F)	93	93	94
DGM Outlet Temperature (°F)	86	86	87
Average DGM Temperature (°F)	89.5	89.5	90.5
Ambient Temperature (°F)	85	85	86
Elapsed Time (min.)	5	5	5
ΔH (inches H ₂ O)	1.80	1.80	1.80
Barometric Pressure (inches Hg)	29.5	29.5	29.5
Pump Vacuum (inches Hg)	19	19	19
K'	0.5885	0.5885	0.5885
V _{cr} (ft ³)	3.718	3.718	3.715
V _{mstd} (ft ³)	3.586	3.596	3.570
Post Test Y _c	1.0368	1.0341	1.0405
Full Test Y _d	1.0141	1.0141	1.0141
% Difference	-2.24	-1.97	-2.60
Average % Difference			-2.27

Airtach Environmental Services, Inc.
Meter Box Full Test Calibration

Date: 11/1/2010

Operator: Jburton

Meter Box ID M-20		Orifice Data					Meter Box ΔH@					Meter Box Y _d					Barometric Pressure (in. Hg.)					Results							
Time	θ (min)	K'	Vacuum		T _{amb}	V _{cr}	V _d	V _{final}	V _{initial}	ΔH	T _i	T _o	T _{avg}	V _{mead}	Q	Y _d	ΔH@												
5.0	5.0	0.3455	22.0	22.0	67	2.220	2.29	958.89	958.89	0.64	73	67	70	2.252	0.444	0.9857	1.766												
5.0	5.0	0.3455	22.0	2.220	67	2.220	2.28	968.89	961.17	0.64	75	69	72.0	2.234	0.444	0.9938	1.788												
5.0	5.0	0.3455	22.0	2.220	67	2.220	2.29	963.46	963.46	0.64	77	70	73.5	2.237	0.444	0.9922	1.777												
5.0	5.0	0.4434	20.0	2.849	67	2.849	2.97	966.67	966.67	1.05	79	72	75.5	2.894	0.570	0.9845	1.740												
5.0	5.0	0.4434	20.0	2.849	67	2.849	2.96	969.63	969.63	1.05	80	72	76.0	2.881	0.570	0.9888	1.753												
5.0	5.0	0.4434	20.0	2.849	67	2.849	2.96	972.59	972.59	1.05	82	74	78.0	2.871	0.570	0.9925	1.760												
5.0	5.0	0.5926	18.0	3.804	68	3.804	4.01	997.01	997.01	1.9	90	81	85.5	3.843	0.761	0.9897	1.759												
5.0	5.0	0.5926	18.0	3.804	68	3.804	4.00	1001.01	1001.01	1.9	93	82	87.5	3.820	0.761	0.9958	1.775												
5.0	5.0	0.5926	18.0	3.804	68	3.804	4.04	1005.05	1005.05	1.9	94	83	88.5	3.851	0.761	0.9878	1.743												
5.0	5.0	0.7995	16.0	5.127	68	5.127	5.35	1011.05	1011.05	3.5	95	84	89.5	5.111	1.026	1.0042	1.834												
5.0	5.0	0.7995	16.0	5.127	69	5.127	5.31	1016.36	1016.36	3.5	98	85	91.5	5.054	1.025	1.0145	1.869												
5.0	5.0	0.7995	16.0	5.127	69	5.127	5.33	1021.69	1021.69	3.5	99	86	92.5	5.064	1.025	1.0125	1.858												
Average															0.9952														

Nomenclature	
K'	Critical Orifice Coefficient
T _{amb}	Ambient Temperature (°F)
V _{cr}	Volume Through Orifice (scf)
V _d	Gas Meter Volume (ft ³)
ΔH	Orifice Pressure Differential (in. H ₂ O)
T _i	Meter Inlet Temperature (°F)
T _o	Meter Outlet Temperature (°F)
T _{avg}	Average Meter Box Temperature (°F)
V _{mead}	Volume Metered Standardized (scf)
Q	Flow Rate (scfm)
Y _d	Meter Correction Factor (dimensionless)
ΔH@	ΔH yielding 0.76 scfm

Vacuum Gauges (in. Hg.)		Thermometers (°F)		
Standard V	Vacuum Gauge	Chr. No.	Chr. No.	Chr. No.
5	5.0	32	31	3
10	10.0	50	50	31
15	15.0	100	100	49
20	20.0	150	151	100
25	25.0	212	213	150
		250	251	213
		300	301	251
		350	352	301
		400	400	351
		500	501	402
		600	601	501
			602	602

$$V_{cr} = K' \cdot P_o \cdot \theta \cdot (T_{amb} + 460)^{-0.5}$$

$$V_{mead} = 17.64 \cdot V_d \cdot (P_o \cdot (T_{i,j} + 460) / (T_{o,j} + 460))$$

$$Q = V_{cr} / \theta$$

$$Y_d = V_{cr} / V_{mead}$$

$$\Delta H(\theta) = 0.319 \cdot \Delta H \cdot (T_{i,j} + 460) \cdot \theta^2 / P_o \cdot Y_d^2 \cdot V_m^2$$

Airtech Environmental Services Meter Post Calibration

Average Field Sample Rate (ΔH)	1.500	Date	8/8/2011
Highest Field Vacuum (inches Hg)	5	Client	BREC
Critical Orifice ID	AA-63	Project No.	3648
Orifice Flow Rate (cfm)	0.766	Meter ID	M-20

	Run 1	Run 2	Run 3
Initial Volume (ft ³)	825.60	829.43	833.26
Final Volume (ft ³)	829.43	833.26	837.08
Volume Metered (ft ³)	3.83	3.83	3.82
DGM Inlet Temperature (°F)	90	90	90
DGM Outlet Temperature (°F)	84	84	84
Average DGM Temperature (°F)	87.0	87.0	87.0
Ambient Temperature (°F)	90	89	88
Elapsed Time (min.)	5	5	5
ΔH (inches H ₂ O)	1.80	1.80	1.80
Barometric Pressure (inches Hg)	29.5	29.5	29.5
Pump Vacuum (inches Hg)	18	18	18
K'	0.5885	0.5885	0.5885
V _{cr} (ft ³)	3.701	3.705	3.708
V _{mstd} (ft ³)	3.660	3.660	3.650
Post Test Y _c	1.0113	1.0122	1.0158
Full Test Y _d	0.9952	0.9952	0.9952
% Difference	-1.62	-1.71	-2.07
Average % Difference			-1.80

Meter Box Initial Calibration

Operator OLEG LAVROV
 Date 10/20/2010

Client XXXXXXXXXX
 Project No MET 30

Meter Box No 207191-A Meter Box Vacuum 1.0 in. H₂O Barometric Pressure 29.02

Q	ΔH	ΔP	Y _{ds}	Standard Meter Gas Volume (cu.ft.)			Meter Box Gas Volume (liters)			Std. Meter Temperature (°F)			Meter Box Temperature (°F)			Calibration Results		
				Initial	Final	V _{ds} Net	Initial	Final	V _d Net	Ambient Temperature	T _{ds} Avg.	T _o Out	In	T _d Avg.	⊙ Time	Y _d	C. factor	
0.035	0.00	0.00	1.0000	0.000	0.362	0.362	0.000	10.214	10.214	10.214	70.0	70.00	77.0	76.50	10.00	1.0148	1.6050	
0.069	0.00	0.00	1.0000	0.000	0.710	0.710	0.000	20.154	20.154	20.154	70.0	70.00	79.0	78.00	10.00	1.0130	1.6050	
0.103	0.00	0.00	1.0000	0.000	1.067	1.067	0.000	30.270	30.270	30.270	71.0	71.00	80.0	80.50	10.00	1.0157	1.6050	

Averages 1.01450 1.60500

Nomenclature	Equations
P _b Barometric Pressure (in. Hg)	
Q Flow Rate (cfm)	
ΔH Orifice Pressure differential (in. H ₂ O)	
ΔP Inlet Pressure Differential (in. H ₂ O)	
V _d Gas Meter Volume - Dry (ft ³)	$Y_d = (Y_{ds}) \left[\frac{V_{ds}}{V_d} \right] \left[\frac{T_d + 460}{T_{ds} + 460} \right] \left[\frac{P_b + \Delta P / 13.6}{P_b + \Delta H / 13.6} \right]$
V _{ds} Standard Meter Volume - Dry (ft ³)	$\Delta H @ = \frac{(0.0319)(\Delta H) \left[\frac{(T_{ds} + 460) \text{⊙}}{(V_{ds})(Y_{ds})} \right]^2}{P_b(T_o + 460)}$
T _d Average Meter Box Temperature (°F)	
T _o Outlet Meter Box Temperature (°F)	
T _{ds} Average Standard Meter Temperature (°F)	
Y _d Meter Correction Factor (unitless)	$Q = \frac{17.64(V_{ds})(P_b)}{(T_{ds} + 460)(\text{⊙})}$
Y _{ds} Standard Meter Correction Factor (unitless)	
ΔH@ Orifice Pressure Differential giving 0.75 cfm of air at 68°F and 29.92 in. Hg (in. H ₂ O)	
⊙ Duration of Run (minutes)	



CAE R2

Meter Box Initial Calibration



Operator OLEG LAVROV

Project No MET 30

Date 10/20/2010

Meter Box No 207191-B Meter Box Vacuum 1.0 in. H₂O

Barometric Pressure 29.02

Q	ΔH	ΔP	Y _{ds}	Standard Meter Gas Volume (cu.ft.)		Meter Box Gas Volume (liters)		Std. Meter Temperature (°F)		Meter Box Temperature (°F)			Calibration Results			
				Initial	Final	V _{ds} Net	Initial	Final	V _d Net	Ambient Temperature	T _{ds} Avg.	In	T _o Out	T _d Avg.	⊕ Time	Y _d
0.035	0.00	0.00	1.0000	0.000	0.358	0.358	0.000	10.363	71.0	71.00	78.0	79.0	78.50	10.00	0.9929	1.6650
0.069	0.00	0.00	1.0000	0.000	0.718	0.718	0.000	20.914	72.0	72.00	81.0	82.0	81.50	10.00	0.9896	1.6650
0.102	0.00	0.00	1.0000	0.000	1.063	1.063	0.000	31.051	72.0	72.00	84.0	85.0	84.50	10.00	0.9925	1.6650

Averages 0.99167 1.66500

Nomenclature	Equations
P _b Barometric Pressure (in. Hg)	
Q Flow Rate (cfm)	
ΔH Orifice Pressure differential (in. H ₂ O)	
ΔP Inlet Pressure Differential (in. H ₂ O)	
V _d Gas Meter Volume - Dry (ft ³)	$Y_d = (Y_{ds}) \left[\frac{V_{ds}}{V_d} \right] \left[\frac{T_d + 460}{T_{ds} + 460} \right] \left[\frac{P_b + \Delta P / 13.6}{P_b + \Delta H / 13.6} \right]$
V _{ds} Standard Meter Volume - Dry (ft ³)	$\Delta H @ = \frac{(0.0319)(\Delta H)}{P_b(T_o + 460)} \left[\frac{(T_{ds} + 460)(\oplus)}{(V_{ds})(Y_{ds})} \right]^2$
T _d Average Meter Box Temperature (°F)	$Q = \frac{17.64(Y_{ds})(P_b)}{(T_{ds} + 460)(\oplus)}$
T _o Outlet Meter Box Temperature (°F)	
T _{ds} Average Standard Meter Temperature (°F)	
Y _d Meter Correction Factor (unitless)	
Y _{ds} Standard Meter Correction Factor (unitless)	
ΔH@ Orifice Pressure Differential giving 0.75 cfm of air at 66°F and 29.92 in. Hg (in. H ₂ O)	
⊕ Duration of Run (minutes)	



Meter Box - Pyrometer Calibration Sheet

Meter Box No: 207191

Office: _____

Calibrated by: OLEG LAVROV

Client: _____

Date: 10/20/10

Job No: _____

Temperature Scale Used: Fahrenheit

Type of Calibration: Full-Test

Calibration Reference Settings (°F)	Pyrometer Reading for each Channel (°F)						
	1	2	3	4	5	6	7
	Stack	Traps	HSL	Imp Out	Aux	DGM In	DGM Out
50	50	52	51				
100	100	102	101				
150	150	152	151				
200	200	202	201				
250	250	252	251				
300	300	302	301				
350	350	352	350				
400	400	402	401				
450	451	452	451				
500	501	502	501				
550	551	552	551				
600	601	602	601				

Tolerance = ±2°F difference from reference setting.

Calibration Reference Information

Reference Used: <u>Omega CL23A</u>	Serial No: <u>T-225950</u>
Calibrated By: <u>JH Metrology</u>	Exp. Date: <u>8/17/2011</u>
Calibration Report No: <u>1000150487</u>	

Meter Box - Pyrometer Calibration Sheet

Meter Box No: 207191

Office: Rentals

Calibrated by: W. Berry

Client: _____

Date: 1/13/11

Job No: _____

Temperature Scale Used: Fahrenheit

Type of Calibration: Post-Test

Calibration Reference Settings (°F)	Pyrometer Reading for each Channel (°F)							
	1 Stack	2 Traps	3 Heated Line	4 Aux 1	5 Aux 2			
50	49	49	50	50	50			
100	99	99	100	100	100			
150	149	150	150	150	150			
200	199	200	200	200	200			
250	249	250	250	250	250			
300	299	300	300	300	300			
350	349	350	350	350	350			
400	399	400	400	400	400			
450	449	450	450	450	450			
500	499	500	500	500	500			
550	549	550	550	550	550			
600	599	600	600	600	600			

Tolerance = ±2°F difference from reference setting.

Calibration Reference Information

Reference Used: Tegam

Serial No: T-242231

Calibrated By: JH Metrology

Exp. Date: 11/24/2011

Calibration Report No: 1000152056



Airtech Environmental Services Meter Post Calibration

Average Field Sample Rate (lpm)	0.500	Date	7/22/2011
Highest Field Vacuum (inches Hg)		Client	BREC
Critical Orifice ID	.5LPM	Project No.	3648
Orifice Flow Rate (lpm)	0.4375	Meter ID	207191-A

	Run 1	Run 2	Run 3
Initial Volume (l)	0.00	4.375	8.704
Final Volume (l)	4.375	8.704	12.956
Volume Metered (l)	4.375	4.329	4.252
DGM Inlet Temperature (°F)	87	86	86
DGM Outlet Temperature (°F)	87	86	86
Average DGM Temperature (°F)	87.0	86.0	86.0
Ambient Temperature (°F)	78	78	78
Elapsed Time (min.)	10	10	10
ΔH (inches H ₂ O)	0.40	0.40	0.40
Barometric Pressure (inches Hg)	29.5	29.5	29.5
Pump Vacuum (inches Hg)	25	25	25
K'	0.0120	0.0120	0.0120
Vcr (l)	4.322	4.322	4.322
Vmstd (l)	4.166	4.130	4.057
Post Test Yc	1.0373	1.0464	1.0654
Full Test Yd	1.0145	1.0145	1.0145
% Difference	-2.25	-3.15	-5.02
Average % Difference			-3.47

Airtech Environmental Services Meter Post Calibration

Average Field Sample Rate (lpm)	0.500	Date	7/22/2011
Highest Field Vacuum (inches Hg)		Client	BREC
Critical Orifice ID	.5LPM	Project No.	3648
Orifice Flow Rate (lpm)	0.4475	Meter ID	207191-B

	Run 1	Run 2	Run 3
Initial Volume (l)	0.00	4.475	9.018
Final Volume (l)	4.475	9.018	13.576
Volume Metered (l)	4.475	4.543	4.558
DGM Inlet Temperature (°F)	89	89	88
DGM Outlet Temperature (°F)	89	89	88
Average DGM Temperature (°F)	89.0	89.0	88.0
Ambient Temperature (°F)	78	78	78
Elapsed Time (min.)	10	10	10
ΔH (inches H ₂ O)	0.30	0.30	0.30
Barometric Pressure (inches Hg)	29.5	29.5	29.5
Pump Vacuum (inches Hg)	24	24	24
K'	0.0120	0.0120	0.0120
Vcr (l)	4.322	4.322	4.322
Vmstd (l)	4.245	4.309	4.332
Post Test Yc	1.0181	1.0029	0.9977
Full Test Yd	0.99167	0.9917	0.9917
% Difference	-2.67	-1.13	-0.61
Average % Difference			-1.47

Meter Box Full Test Calibration

R-20098

DATE: 7/10/2011

Operator: Joe Ward

Meter Box No. DB30B-0711-2019		Meter Box H@:		Meter Box Gas		Meter Box Yd		Meter Box		Barometric Pressure:		
#1		Volume		Volume (ft ³)		Std. Meter Temperature (PF)		Temperature (PF)		29.79		
Q	P	H	Yds	Initial	Final	Vf	Inlet	Outlet	Avg.	Time	Yd	H@
0.04	-0.30	0.00	1.0000	0.0	1.000	1.018	75.0	75.0	75.0	26.40	1.0124	0.0000
0.04	-0.30	0.00	1.0000	0.0	1.000	1.019	75.0	75.0	75.0	26.38	1.0115	0.0000
0.02	-0.30	0.00	1.0000	0.0	.520	.536	75.0	75.0	75.0	22.14	1.0035	0.0000
0.02	-0.30	0.00	1.0000	0.0	.500	.516	75.0	75.0	75.0	22.09	1.0041	0.0000
0.02	-0.30	0.00	1.0000	0.0	.500	.523	76.0	76.0	76.0	32.22	1.0067	0.0000
0.02	-0.30	0.00	1.0000	0.0	.500	.524	76.0	76.0	76.0	32.20	1.0048	0.0000
AVERAGE											1.0072	0.0000

Vacuum Gauge

(in. Hg)	Gauge
5.0	5.5
10.0	10.5
15.0	16.0
20.0	21.0

Millennium Instruments Inc.
 2402 Springridge Drive unit A
 Spring Grove IL. 60081
 PHONE#(815)675-3225
 FAX#(815)675-6965
 E-mail millennium@millinst.com
 www.millinst.com

New Ashtead

Meter Box Full Test Calibration

R-20078

DATE: 7/11/2011

Operator: Joe Ward

Meter Box No: DB30B-0711-2019		Meter Box H@: 0.0000		Meter Box Yd 0.9985		Barometric Pressure: 29.69							
Q	P	Standard Meter Gas Volume		Meter Box Gas Volume (ft ³)		Std. Meter Temperature (PF)		Meter Box Temperature (PF)		Time	Yd	H@	
		Initial	Final	Vf	Vf	Inlet	Outlet	Avg.	Avg.				
0.03	-0.30	0.00	1.000	1.000	1.024	1.024	75.0	75.0	92.0	92.0	30.56	1.0083	0.0000
0.03	-0.30	0.00	1.000	1.000	1.025	1.025	75.0	75.0	92.0	92.0	30.48	1.0074	0.0000
0.02	-0.30	0.00	.500	.500	.518	.518	75.0	75.0	94.0	94.0	22.10	1.0003	0.0000
0.02	-0.30	0.00	.500	.500	.518	.518	75.0	75.0	94.0	94.0	21.90	1.0003	0.0000
0.01	-0.30	0.00	.500	.500	.528	.528	76.0	76.0	98.0	98.0	38.94	0.9866	0.0000
0.01	-0.30	0.00	.500	.500	.527	.527	76.0	76.0	98.0	98.0	38.85	0.9884	0.0000
AVERAGE											0.9985	0.0000	

Vacuum Gauge

(in. Hg)	Gauge
5.0	5.0
10.0	10.0
15.0	15.0
20.0	20.0

Millennium Instruments Inc.
 2402 Springridge Drive unit A
 Spring Grove IL. 60081
 PHONE#(815)675-3225
 FAX#(815)675-6965
 E-mail millennium@millinst.com
 www.millinst.com

R-20078

Pyrometer Calibration Sheet

Pyrometer No.:001

Office: Spring Grove
Client: Ashtead Technology Rentals
Job or Reference No.:DB30B-0711-2019

Temperature Scale Used

Fahrenheit
 Celsius

Full Test
 Post Test

Calibration Reference Settings for Fahrenheit Scale	Pyrometer Reading	Calibration Reference Settings for Celsius Scale
50° F	50° F	10°C
100° F	100° F	38°C
150° F	150° F	66°C
200° F	200° F	93°C
250° F	250° F	121°C
300° F	300° F	149°C
350° F	350° F	177°C
400° F	400° F	204°C
450° F	450° F	232°C
500° F	500° F	260°C
550° F	550° F	288°C
600° F	600° F	316°C

Method 30B Post-Test Meter Calibration

Average Field Sample Rate (lpm)	0.5	Date	8/8/2011
Highest Field Vacuum (inches Hg)	10.0	Client	BREC
Critical Orifice ID	.5LPM	Project No.	3648
Orifice Flow Rate (lpm)	0.473	Meter ID	R-20078A

	Run 1	Run 2	Run 3	
Initial Volume (l³)	0.000	4.676	9.411	
Final Volume (l³)	4.676	9.411	14.181	
Volume Metered (l³)	4.676	4.735	4.770	
DGM Temperature (°F)	106	108	112	
Ambient Temperature (°F)	87	88	88	
Elapsed Time (min.)	10.0	10.0	10.0	
Setting (l/min)	0.4	0.4	0.4	
Barometric Pressure (inches Hg)	29.50	29.50	29.50	
Pump Vacuum (inches Hg)	20.0	20.0	20.0	
K'	0.012	0.012	0.012	
Vcr (l³)	4.285	4.281	4.281	
Vmstd (l³)	4.303	4.342	4.344	
Post Test Yc	0.99572	0.98589	0.98555	
Full Test Yd	1.0072	1.0072	1.0072	
% Difference	1.14	2.12	2.15	
	Average Difference		1.80	

Method 30B Post-Test Meter Calibration

Average Field Sample Rate (lpm)	0.5	Date	8/8/2011
Highest Field Vacuum (inches Hg)	10.0	Client	BREC
Critical Orifice ID	.5LPM	Project No.	3648
Orifice Flow Rate (lpm)	0.487	Meter ID	R-20078B

	Run 1	Run 2	Run 3	
Initial Volume (l³)	0.000	4.891	9.779	
Final Volume (l³)	4.891	9.779	14.623	
Volume Metered (l³)	4.891	4.888	4.844	
DGM Temperature (°F)	116	116	115	
Ambient Temperature (°F)	87	87	86	
Elapsed Time (min.)	10.0	10.0	10.0	
Setting (l/min)	0.5	0.5	0.5	
Barometric Pressure (inches Hg)	29.50	29.50	29.50	
Pump Vacuum (inches Hg)	18.0	18.0	18.0	
K'	0.012	0.012	0.012	
Vcr (l³)	4.285	4.285	4.289	
Vmstd (l³)	4.424	4.422	4.389	
Post Test Yc	0.96853	0.96912	0.97712	
Full Test Yd	0.9985	0.9985	0.9985	
% Difference	3.00	2.94	2.14	
	Average Difference		2.69	

Airtech Environmental Services, Inc.
30B Meter Box Full Test Calibration

Date: 1/5/2011

Operator: S. Behanish

Meter Box	M-25 A	Meter Box Y _d	0.9994	Barometric Pressure (in. Hg.)	24.57								
Time	Orifice Data				Meter Box Data				Results				
	K'	Vacuum	T _{amb}	V _{cr}	V _{inlet}	V _{final}	V _d	LPM	T _{in}	V _{inlet}	Q	Y _d	ΔH@
θ (min)	0.012	15.0	75	3.610	0.00	4.84	4.84	0.48	115	3.654	0.361	0.9880	1.544
10.0	0.012	15.0	75	3.610	4.84	9.63	4.79	0.48	115	3.616	0.361	0.9983	1.560
10.0	0.012	15.0	75	3.610	9.63	14.47	4.84	0.48	116	3.647	0.361	0.9897	1.547
10.0	0.028	14.0	75	8.422	0.00	10.95	10.95	1.10	115	8.281	0.842	1.0171	0.683
10.0	0.028	14.0	75	8.422	10.95	22.03	11.08	1.11	115	8.379	0.842	1.0051	0.675
10.0	0.028	14.0	75	8.422	22.03	33.00	10.97	1.10	116	8.282	0.842	1.0170	0.683
10.0	0.051	12.5	76	15.326	0.00	20.30	20.30	2.03	116	15.368	1.533	0.9973	0.368
10.0	0.051	12.5	77	15.312	20.30	40.68	20.38	2.04	116	15.429	1.531	0.9925	0.367
10.0	0.051	12.5	78	15.298	40.68	61.10	20.42	2.04	116	15.459	1.530	0.9896	0.367
											Average	0.9994	0.866

Nomenclature	
K'	Critical Orifice Coefficient
T _{amb}	Ambient Temperature (°F)
V _{cr}	Volume Through Orifice (L)
V _d	Gas Meter Volume (L)
ΔH	Orifice Pressure Differential (in. H ₂ O)
T _i	Meter Inlet Temperature (°F)
T _o	Meter Outlet Temperature (°F)
T _{avg}	Average Meter Box Temperature (°F)
V _{m, std}	Volume Metered Standardized (L)
Q	Flow Rate (scfm)
Y _d	Meter Correction Factor (dimensionless)
ΔH@	ΔH yielding 0.75 scfm

Vacuum Gauge (in. Hg.)		Thermometers (°F)			
Standard	Vacuum Gauge	Standard	Chr. No.	Chr. No.	Chr. No.
			Aux 1	Aux 2	Aux 2
5	5.0	32	34	34	34
10	10.0	50	51	51	51
15	15.0	100	102	102	102
20	20.0	150	152	152	152
25	25.0	212	214	214	214
		250	252	252	252
		300	302	302	302
		350	352	352	352
		400	402	402	402
		500	502	502	502
		600	602	602	602

$$V_m = K' \cdot E_o \cdot \theta \cdot \sqrt{\frac{P_b}{(T_{in}) + 460}} \cdot 0.5$$

$$V_{m, std} = 17.64 \cdot V_d \cdot \sqrt{\frac{P_b}{(T_{in}) + 460}} \cdot \sqrt{\frac{P_b + (\Delta H / 13.6)}{P_b + 460}}$$

$$Q = V_{cr} \cdot \theta$$

$$Y_d = V_{cr} / V_{m, std}$$

$$\Delta H@ = \frac{0.319 \cdot \Delta H \cdot (T_{avg} + 460) \cdot \theta^2}{P_b \cdot Y_d^2 \cdot V_m^2}$$

Airtech Environmental Services Meter Post Calibration

Average Field Sample Rate (lpm)	0.500	Date	8/12/2011
Highest Field Vacuum (inches Hg)	10	Client	BREC
Critical Orifice ID	.5LPM	Project No.	3648
Orifice Flow Rate (lpm)	0.4486	Meter ID	M-25-A

	Run 1	Run 2	Run 3
Initial Volume (l)	0.00	4.486	9.072
Final Volume (l)	4.486	9.072	13.869
Volume Metered (l)	4.486	4.586	4.797
DGM Inlet Temperature (°F)	94	99	104
DGM Outlet Temperature (°F)	94	99	104
Average DGM Temperature (°F)	94.0	99.0	104.0
Ambient Temperature (°F)	79	78	79
Elapsed Time (min.)	10	10	10
ΔH (inches H ₂ O)	0.40	0.40	0.40
Barometric Pressure (inches Hg)	29.5	29.5	29.5
Pump Vacuum (inches Hg)	18	18	18
K'	0.0120	0.0120	0.0120
Vcr (l)	4.318	4.322	4.318
Vmstd (l)	4.218	4.273	4.430
Post Test Yc	1.0237	1.0113	0.9746
Full Test Yd	0.9994	0.9994	0.9994
% Difference	-2.43	-1.19	2.48
Average % Difference			-0.38

Airtech Environmental Services, Inc.
30B Meter Box Full Test Calibration

Date: 3/29/2011

Operator: lburp21

Meter Box	M-25B	Meter Box Y _d	1.0017	Barometric Pressure (in. Hg.)	29.50								
Meter Box Data													
Time	Orifice Data					Results							
θ (min)	K'	Vacuum	T _{amb}	V _{cr}	V _{initial}	V _{final}	V _d	LPM	T _m	V _{meas}	Q	Y _d	ΔH@
10.0	0.012	21.0	70	4.354	0.000	4.634	4.634	0.46	100	4.311	0.435	1.0100	1.293
10.0	0.012	21.0	70	4.354	4.634	9.253	4.619	0.46	99	4.305	0.435	1.0115	1.299
10.0	0.012	21.0	70	4.354	9.253	13.827	4.574	0.46	98	4.271	0.435	1.0196	1.322
10.0	0.019	20.0	68	6.907	0.000	7.530	7.530	0.75	97	7.048	0.691	0.9800	0.794
10.0	0.019	20.0	69	6.901	7.530	14.961	7.431	0.74	96	6.968	0.690	0.9904	0.803
10.0	0.019	20.0	70	6.894	14.961	22.428	7.467	0.75	96	7.002	0.689	0.9846	0.806
10.0	0.028	20.0	69	10.169	0.000	10.753	10.753	1.08	96	10.091	1.017	1.0078	0.560
10.0	0.028	20.0	69	10.169	10.753	21.576	10.823	1.08	96	10.157	1.017	1.0012	0.552
10.0	0.028	20.0	68	10.179	21.576	32.297	10.721	1.07	95	10.079	1.018	1.0099	0.557
10.0	0.041	19.0	68	14.905	0.000	15.482	15.482	1.55	95	14.572	1.491	1.0228	0.387
10.0	0.041	19.0	68	14.905	15.482	30.965	15.483	1.55	95	14.573	1.491	1.0228	0.387
10.0	0.041	19.0	68	14.905	30.965	46.450	15.485	1.55	95	14.556	1.491	1.0240	0.388
											Average	1.0017	0.887

Nomenclature	
K'	Critical Orifice Coefficient
T _{amb}	Ambient Temperature (°F)
V _{cr}	Volume Through Orifice (L)
V _d	Gas Meter Volume (L)
ΔH	Orifice Pressure Differential (in. H ₂ O)
T _i	Meter Inlet Temperature (°F)
T _o	Meter Outlet Temperature (°F)
T _{avg}	Average Meter Box Temperature (°F)
V _{meas}	Volume Metered Standardized (L)
Q	Flow Rate (scfm)
Y _d	Meter Correction Factor (dimensionless)
ΔH@	ΔH yielding 0.75 scfm

Vacuum Gauge (in. Hg.)		Thermometers (°F)			Equations	
Standard	Vacuum Gauge	Ch. No.	Ch. No.	Ch. No.		
5	5.0	1	probe		$V_m = K' \cdot P_b \cdot \theta$	
10	10.0	32	32		$(T_{meas} + 460) \wedge 0.5$	
15	15.0	50	49		$V_{meas} = 17.64 \cdot V_d \cdot (P_b + (\Delta H / 13.6))$	
20	20.0	100	101		$(T_{m_i} + 460)$	
25	25.0	150	152		$Q = V_m / \theta$	
		212	213		$Y_d = V_m / V_{meas}$	
		250	251		$\Delta H@ = .0319 \cdot \Delta H + (T_{meas} + 460) \cdot \theta \wedge 2$	
		300	301		$P_b \cdot Y_d \wedge 2 \cdot V_m \wedge 2$	
		350	351			
		400	400			
		500	501			
		600	601			
			599			

Airtech Environmental Services

Meter Post Calibration

Average Field Sample Rate (lpm)	0.500	Date	8/12/2011
Highest Field Vacuum (inches Hg)	10	Client	BREC
Critical Orifice ID	.5LPM	Project No.	3648
Orifice Flow Rate (lpm)	0.4864	Meter ID	M-25-B

	Run 1	Run 2	Run 3
Initial Volume (l)	0.00	4.864	9.786
Final Volume (l)	4.864	9.786	14.644
Volume Metered (l)	4.864	4.922	4.858
DGM Inlet Temperature (°F)	113	115	116
DGM Outlet Temperature (°F)	113	115	116
Average DGM Temperature (°F)	113.0	115.0	116.0
Ambient Temperature (°F)	82	81	81
Elapsed Time (min.)	10	10	10
ΔH (inches H₂O)	0.40	0.40	0.40
Barometric Pressure (inches Hg)	29.5	29.5	29.5
Pump Vacuum (inches Hg)	19	19	19
K'	0.0120	0.0120	0.0120
V_{cr} (l)	4.306	4.310	4.310
V_{mstd} (l)	4.422	4.459	4.393
Post Test Y_c	0.9738	0.9666	0.9810
Full Test Y_d	1.0017	1.0017	1.0017
% Difference	2.79	3.51	2.07
Average % Difference			2.79

Meter Box Full Test Calibration

M26-

DATE: 7/8/2011

Operator: Joe Ward

Meter Box No: DB30B-0711-2018		Meter Box H@:		Meter Box Gas		Meter Box Yd		Meter Box Pressure:			
		0.0000		0.9958		29.78					
#1	Standard Meter Gas		Volume (ft ³)		Std. Meter Temperature (pF)		Meter Box Temperature (pF)		H@		
	Initial	Final	Vf		Inlet	Outlet	Avg.	Time		Yd	
0.04	0.0	1.000	1.000	1.015	1.015	76.0	76.0	81.0	27.04	0.9951	0.0000
0.04	0.0	1.000	1.000	1.014	1.014	76.0	76.0	80.0	27.06	0.9943	0.0000
0.02	0.0	.500	.500	.503	.503	77.0	77.0	80.0	29.91	1.0003	0.0000
0.02	0.0	.500	.500	.502	.502	77.0	77.0	80.0	29.52	1.0023	0.0000
0.03	0.0	.500	.500	.507	.507	78.0	78.0	81.0	17.92	0.9924	0.0000
0.03	0.0	.500	.500	.508	.508	78.0	78.0	81.0	17.79	0.9905	0.0000
AVERAGE										0.9958	0.0000

Millennium Instruments Inc.
 2402 Springridge Drive unit A
 Spring Grove IL. 60081
 PHONE#(815)675-3225
 FAX#(815)675-6965
 E-mail millennium@millinst.com
 www.millinst.com

Vacuum Gauge

(in. Hg)	Gauge
5.0	5.5
10.0	10.5
15.0	16.0
20.0	21.0
25.0	26.0

Meter Box Full Test Calibration

DATE: 7/10/2011

M-26

Operator: Joe Ward

Meter Box No. DB30B-0711-2018		Meter Box H@:		Meter Box Gas		Meter Box Gas		Meter Box Yd		Meter Box		Barometric Pressure:				
		Volume		Volume (ft ³)		Temperature (pF)		Temperature (pF)				29.75				
#2	Q	P	H	Yds	Initial	Final	Vf	Initial	Final	Vf	Inlet	Outlet	Avg.	Time	Yd	H@
	0.01	-0.30	0.00	1.0000	0.0	.280	.280	.000	.294	.294	75.0	75.0	75.0	18.66	0.9834	0.0000
	0.01	-0.30	0.00	1.0000	0.0	.285	.285	0.000	.299	.299	75.0	75.0	75.0	18.64	0.9842	0.0000
	0.03	-0.30	0.00	1.0000	0.0	1.000	1.000	.000	1.033	1.033	75.0	75.0	75.0	29.14	1.0014	0.0000
	0.03	-0.30	0.00	1.0000	0.0	1.000	1.000	.000	1.032	1.032	75.0	75.0	75.0	29.10	1.0023	0.0000
	0.02	-0.30	0.00	1.0000	0.0	.500	.500	.000	.527	.527	75.0	75.0	75.0	22.89	0.9850	0.0000
	0.02	-0.30	0.00	1.0000	0.0	.500	.500	.000	.527	.527	75.0	75.0	75.0	22.80	0.9850	0.0000
AVERAGE													0.9902	0.9902	0.0000	

Millennium Instruments Inc.
 2402 Springridge Drive unit A
 Spring Grove IL. 60081
 PHONE#(815)675-3225
 FAX#(815)675-6965
 E-mail millennium@millinst.com
 www.millinst.com

Vacuum Gauge

(in. Hg)	Gauge
5.0	5.0
10.0	10.0
15.0	15.0
20.0	20.0

Pyrometer Calibration Sheet

Pyrometer No.:001

Office: Spring Grove

Client: Airtech Environmental

Job or Reference No.:DB30B-0711-2018

Temperature Scale Used

Fahrenheit
 Celsius

Full Test
 Post Test

Calibration Reference Settings for Fahrenheit Scale	Pyrometer Reading	Calibration Reference Settings for Celsius Scale
50° F	50° F	10°C
100° F	100° F	38°C
150° F	150° F	66°C
200° F	200° F	93°C
250° F	250° F	121°C
300° F	300° F	149°C
350° F	350° F	177°C
400° F	400° F	204°C
450° F	450° F	232°C
500° F	500° F	260°C
550° F	550° F	288°C
600° F	600° F	316°C

Method 30B Post-Test Meter Calibration

Average Field Sample Rate (lpm)	0.5	Date	8/8/2011
Highest Field Vacuum (inches Hg)	10.0	Client	BREC
Critical Orifice ID	.5LPM	Project No.	3648
Orifice Flow Rate (lpm)	0.479	Meter ID	M-26 A

	Run 1	Run 2	Run 3	
Initial Volume (l³)	0.000	4.798	9.564	
Final Volume (l³)	4.798	9.564	14.362	
Volume Metered (l³)	4.798	4.766	4.798	
DGM Temperature (°F)	104	105	107	
Ambient Temperature (°F)	88	87	88	
Elapsed Time (min.)	10.0	10.0	10.0	
Setting (l/min)	0.4	0.4	0.4	
Barometric Pressure (inches Hg)	29.50	29.50	29.50	
Pump Vacuum (inches Hg)	19.0	19.0	19.0	
K'	0.012	0.012	0.012	
Vcr (l³)	4.281	4.285	4.281	
Vmstd (l³)	4.431	4.394	4.408	
Post Test Yc	0.96609	0.97519	0.97123	
Full Test Yd	0.9958	0.9958	0.9958	
% Difference	2.98	2.07	2.47	
	Average Difference		2.51	

Method 30B Post-Test Meter Calibration

Average Field Sample Rate (lpm)	0.5	Date	8/8/2011
Highest Field Vacuum (inches Hg)	10.0	Client	BREC
Critical Orifice ID	.5LPM	Project No.	3648
Orifice Flow Rate (lpm)	0.480	Meter ID	M-26 B

	Run 1	Run 2	Run 3	
Initial Volume (l³)	0.000	4.802	9.592	
Final Volume (l³)	4.802	9.592	14.401	
Volume Metered (l³)	4.802	4.790	4.809	
DGM Temperature (°F)	106	108	107	
Ambient Temperature (°F)	88	87	88	
Elapsed Time (min.)	10.0	10.0	10.0	
Setting (l/min)	0.4	0.4	0.4	
Barometric Pressure (inches Hg)	29.50	29.50	29.50	
Pump Vacuum (inches Hg)	20.0	20.0	20.0	
K'	0.012	0.012	0.012	
Vcr (l³)	4.281	4.285	4.281	
Vmstd (l³)	4.419	4.393	4.418	
Post Test Yc	0.96871	0.97546	0.96901	
Full Test Yd	0.9902	0.9902	0.9902	
% Difference	2.17	1.49	2.14	
	Average Difference		1.93	



APEX INSTRUMENTS METER CONSOLE CALIBRATION

Meter Console Information

Console Model	XC-260	Console Serial Number	0905008-A	Encoder Model	HEDS-9100-F00
Gas Meter Model	SK25	Totalizer Scale Factor (Initial)	1.0000	Totalizer Model	RED LION
Gas Meter Serial#	8005093	Totalizer Scale Factor (Final)	0.9728	Temp Display Model	JENCO

Calibration Conditions

WTM ID	539783	Calibration Technician	EW	Calibration Date	16-Aug-10
WTM Cal Factor	1.0001	Barometric Pressure	(Pb) 735.5 mm Hg		

Calibration Data

Run Time	Dry Gas Meter				Wet Test Meter				Standardized Volumes				Results		
	Gas Pressure (P _m) mm H ₂ O	Gas Volume (V _m) liters	Gas Temp (t _m) °C	Totalizer Display	Gas Volume (V _w) liters	Gas Temp (t _w) °C	Totalizer Initial SF (V _{m(stg)}) std liters	Totalizer Final SF (V _{w(stg)}) std liters	Wet Test Meter (V _{w(stg)}) std liters	Totalizer Gamma Final	Totalizer Gamma Variation (Y) (ΔY)	Corrected Flowrate (Q _m) slm			
Run 1 - Initial	0	0	23.33	0.000	780.096	24.0									
Final	0	0	23.33	13.406	793.113	24.0									
Total/Avg	0	0	23.33	13.406	13.017	24.0	12.837	12.488	12.438	0.9960	-0.004	2.49			
Run 2 - Initial	0	0	23.33	13.406	793.113	24.0									
Final	0	0	23.33	26.513	805.870	24.0									
Total/Avg	0	0	23.33	13.107	12.757	24.0	12.551	12.209	12.189	0.9984	-0.002	2.03			
Run 3 - Initial	0	0	23.33	26.513	805.870	24.0									
Final	0	0	23.33	37.917	816.961	24.0									
Total/Avg	0	0	23.33	11.404	11.091	24.0	10.920	10.623	10.597	0.9976	-0.002	1.51			
Run 4 - Initial	0	0	23.33	37.917	816.961	24.0									
Final	0	0	23.89	50.554	829.294	24.0									
Total/Avg	0	0	23.61	12.637	12.333	24.0	12.089	11.760	11.784	1.0020	0.002	0.98			
Run 5 - Initial	0	0	23.89	50.554	829.294	24.0									
Final	0	0	23.89	63.375	841.845	24.0									
Total/Avg	0	0	23.89	12.821	12.551	24.0	12.254	11.920	11.993	1.0060	0.006	0.50			

Average Meter Calibration Factor Y

1.0000

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ±0.02.


I certify that the above Dry Gas Meter was calibrated in accordance with USEPA Methods, CFR 40 Part 61, using a Precision Wet Test Meter, which in turn was calibrated using the Ashtead "Bip" Prover #3789, certificate # 1107, which is traceable to the National Bureau of Standards (N.I.S.T.).

Signature: *Eileen W. [unclear]*

Date: *8/16/10*

R19075

Electronic Totalizer Y vs Standardized Flowrate

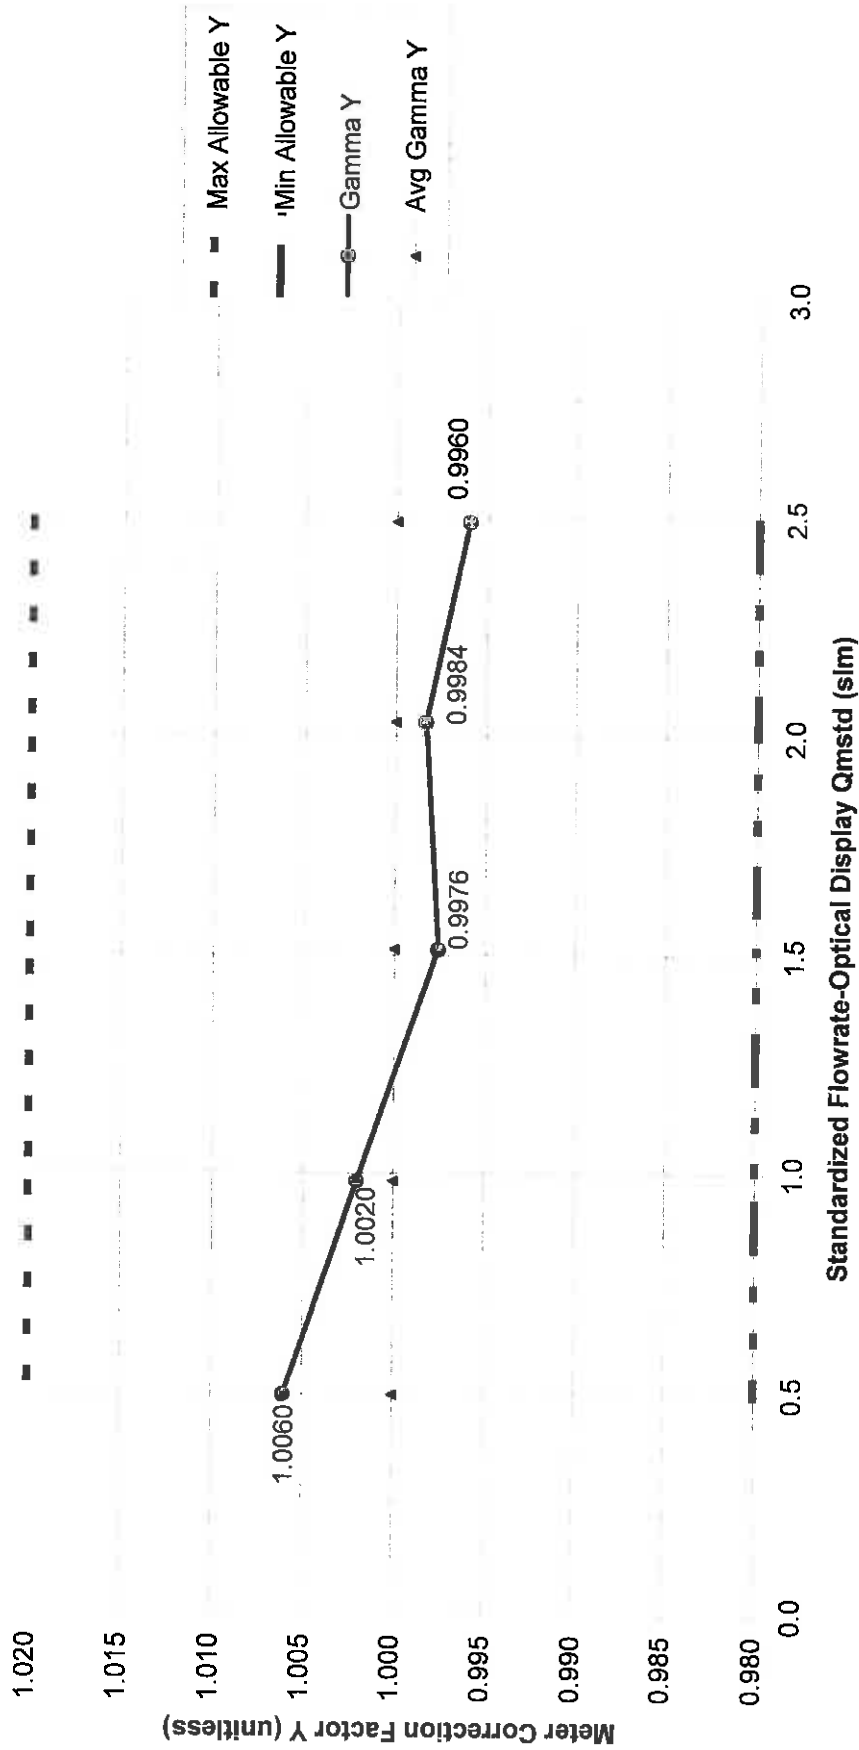

Console Serial: 0905008-A

Airtech Environmental Services Meter Post Calibration

Average Field Sample Rate (lpm)	0.500	Date	8/1/2011
Highest Field Vacuum (inches Hg)	10	Client	BREC
Critical Orifice ID	.5LPM	Project No.	3648
Orifice Flow Rate (lpm)	0.4479	Meter ID	R19075A

	Run 1	Run 2	Run 3
Initial Volume (l)	0.00	4.479	8.984
Final Volume (l)	4.479	8.984	13.48
Volume Metered (l)	4.479	4.51	4.50
DGM Inlet Temperature (°F)	83	84	85
DGM Outlet Temperature (°F)	83	84	85
Average DGM Temperature (°F)	83.0	84.0	85.0
Ambient Temperature (°F)	80	80	80
Elapsed Time (min)	10	10	10
ΔH (inches H ₂ O)	0.40	0.40	0.40
Barometric Pressure (inches Hg)	29.58	29.58	29.58
Pump Vacuum (inches Hg)	22	22	22
K'	0.0120	0.0120	0.0120
Vcr (l)	4.325	4.325	4.325
Vmstd (l)	4.308	4.325	4.313
Post Test Yc	1.0040	1.0000	1.0030
Full Test Yd	1.000	1.0000	1.0000
% Difference	-0.40	0.00	-0.30
Average % Difference			-0.23



APEX INSTRUMENTS METER CONSOLE CALIBRATION

Meter Console Information			
Console Model	XC-260	Console Serial Number	0905008-B
Encoder Model		Encoder Model	HEDS-9100-F00
Gas Meter Model	SK25	Totalizer Scale Factor (Initial)	1.0000
Gas Meter Serial#	8005094	Totalizer Scale Factor (Final)	0.9756
		Temp Display Model	JENCO

Calibration Conditions			
WTM ID	539784	Calibration Technician	EW
WTM Cal Factor	1.0024	Barometric Pressure (Pb)	735.5 mm Hg
			Calibration Date
			16-Aug-10

Run Time	Calibration Data										Results					
	Dry Gas Meter					Wet Test Meter					Standardized Volumes			Totalizer Gamma		Corrected Flowrate
	Gas Pressure (P _m) mm H ₂ O	Gas Volume (V _m) liters	Gas Temp (t _m) °C	Gas Totalizer Display	Gas Volume (V _w) liters	Gas Temp (t _w) °C	Initial SF (V _{m(std)}) std liters	Final SF (V _{w(std)}) std liters	Totalizer Initial SF	Totalizer Final SF	Totalizer Wet Test Meter (V _{w(std)}) std liters	Final Variation (Y)	(ΔY)	(Q _{mp})		
Run 1 - Initial	0	0	23.89	0.000	195.508	24.0										
Final	0	0	24.44	13.356	208.479	24.0										
Total/Avg	0	0	24.17	13.356	12.971	24.0	12.753	12.443	12.422	12.422	0.9984	-0.002				2.49
Run 2 - Initial	0	0	24.44	13.356	208.479	24.0										
Final	0	0	25.00	26.505	221.226	24.0										
Total/Avg	0	0	24.72	13.149	12.747	24.0	12.532	12.227	12.208	12.208	0.9984	-0.002				2.04
Run 3 - Initial	0	0	25.00	26.505	221.226	24.0										
Final	0	0	25.00	37.866	232.244	24.0										
Total/Avg	0	0	25.00	11.361	11.018	24.0	10.818	10.554	10.552	10.552	0.9998	0.000				1.51
Run 4 - Initial	0	0	25.00	37.866	232.244	24.0										
Final	0	0	25.00	50.775	244.775	24.0										
Total/Avg	0	0	25.00	12.909	12.531	24.0	12.292	11.992	12.001	12.001	1.0007	0.001				1.00
Run 5 - Initial	0	0	25.00	50.775	244.775	24.0										
Final	0	0	25.56	64.499	258.111	24.0										
Total/Avg	0	0	25.28	13.724	13.336	24.0	13.056	12.738	12.772	12.772	1.0027	0.003				0.53

Average Meter Calibration Factor Y 1.0000


Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ±0.02.

I certify that the above Dry Gas Meter was calibrated in accordance with USEPA Methods, CFR 40 Part 60, using a Precision Wet Test Meter, which in turn was calibrated using the American Bell Pro'er # 3785, certificate # F107, which is traceable to the National Bureau of Standards (N.I.S.T.).

Signature *[Signature]* Date *8/16/10*

R 19075

Electronic Totalizer Y vs Standardized Flowrate

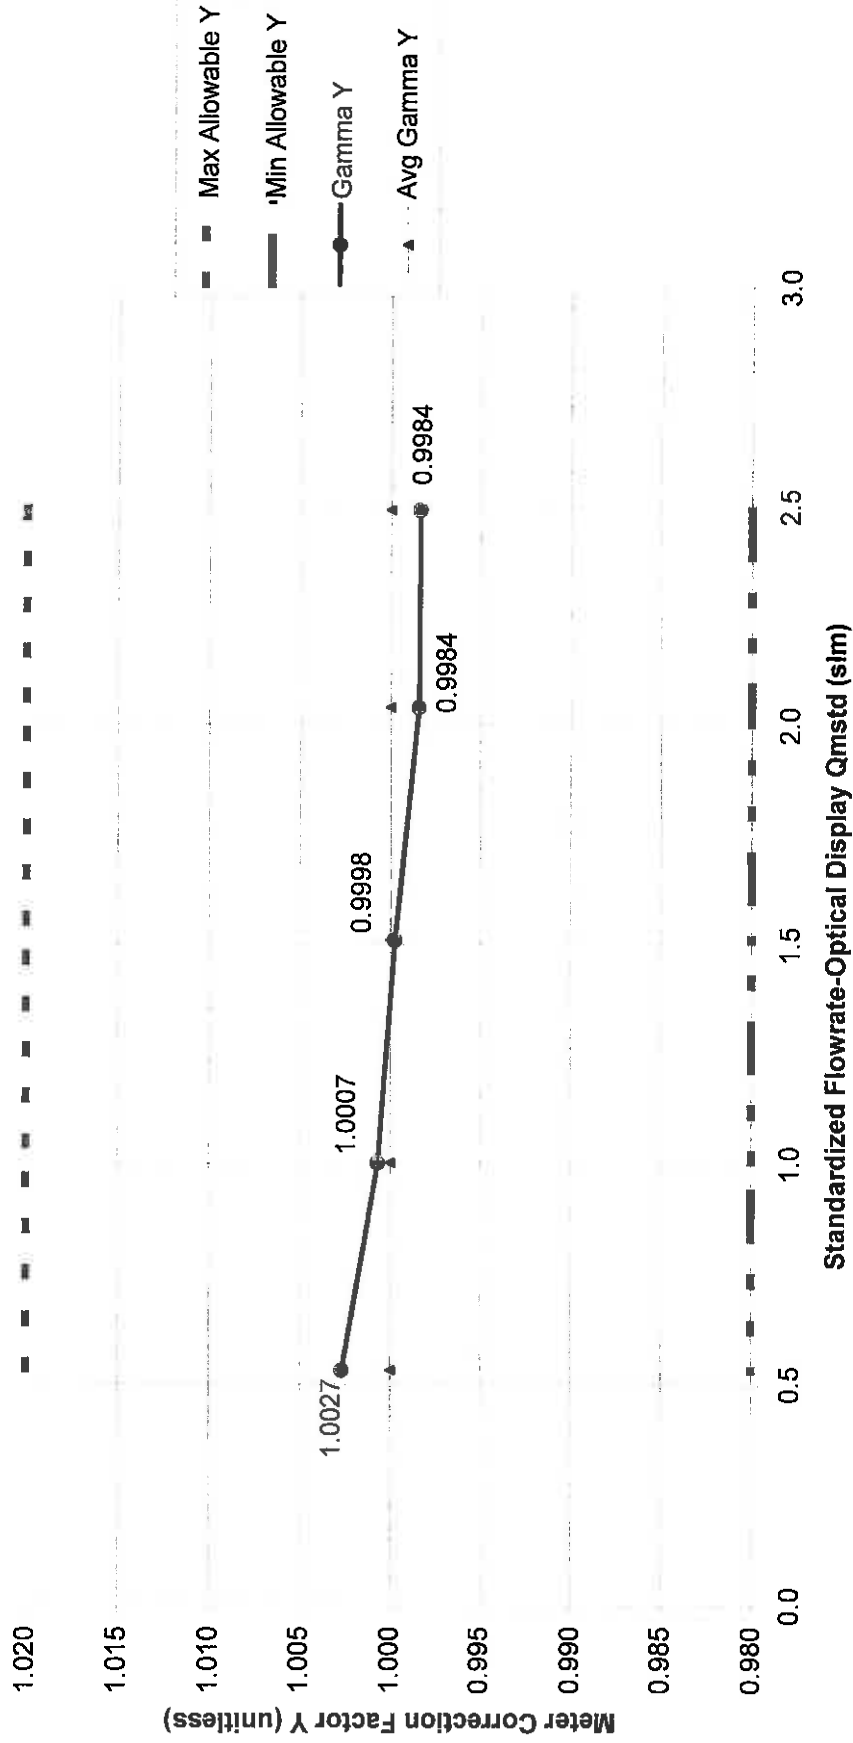

Console Serial: 0905008-B

Airtech Environmental Services Meter Post Calibration

Average Field Sample Rate (lpm)	0.500	Date	8/1/2011
Highest Field Vacuum (inches Hg)	10	Client	BREC
Critical Orifice ID	.5LPM	Project No.	3648
Orifice Flow Rate (lpm)	0.4553	Meter ID	R19075B

	Run 1	Run 2	Run 3
Initial Volume (l)	0.00	4.553	9.078
Final Volume (l)	4.553	9.078	13.65
Volume Metered (l)	4.553	4.53	4.57
DGM Inlet Temperature (°F)	87	87	87
DGM Outlet Temperature (°F)	87	87	87
Average DGM Temperature (°F)	87.0	87.0	87.0
Ambient Temperature (°F)	80	80	80
Elapsed Time (min.)	10	10	10
ΔH (inches H ₂ O)	0.40	0.40	0.40
Barometric Pressure (inches Hg)	29.58	29.58	29.58
Pump Vacuum (inches Hg)	21	21	21
K'	0.0120	0.0120	0.0120
Vcr (l)	4.325	4.325	4.325
Vmstd (l)	4.347	4.321	4.366
Post Test Yc	0.9949	1.0011	0.9908
Full Test Yd	1.000	1.0000	1.0000
% Difference	0.51	-0.11	0.92
Average % Difference			0.44

Airtech Environmental Services, Inc.
S-Type Pitot Tube Inspection Form

Date 1/25/11
Pitot ID AE5-6-2
Operator EA

	Measured	Allowed
Outside Tube Diameter - Dt (inches)	0.250	NA
Base To Opening Distance - Pa (inches)	0.356	NA
Base To Opening Distance - Pb (inches)	0.356	NA
Pa/Dt	1.42	1.05-1.50
Pb/Dt	1.42	1.05-1.50
Angle $\alpha 1$ ($^{\circ}$)	2.7	10
Angle $\alpha 2$ ($^{\circ}$)	2.6	10
Angle B1 ($^{\circ}$)	4	5
Angle B1 ($^{\circ}$)	0.6	5
Opening to Opening Distance Pa+Pb (inches)	0.712	NA
Angle Z ($^{\circ}$)	0.4	NA
z (inches)	0.0050	0.125
Angle W ($^{\circ}$)	0	NA
w (inches)	0.000	0.031

Note Any Damage, Nicks or Dents to the Pitot Tube

Is the Pitot Tube Part of an Assembly Yes
If Yes, Complete the Section Below

Pitot	Measured	Minimum
Distance From Nozzle (inches)	0.75	0.75 in.
Pitot to Thermocouple Distance (inches)	2	2 in.
Pitot to Sample Probe Distance (inches)	6.25	3 in.

Does the Pitot Tube Meet the Above Requirements Yes
Is the Pitot Tube Free of Damage Yes

If Yes to Both, a Pitot Tube Coefficient of 0.84 is Assigned
If No to Either, then the Pitot Tube Must be Calibrated

Airtech Environmental Services, Inc.
S-Type Pitot Tube Inspection Form

Date 1/25/11
Pitot ID AE-5-6-8
Operator EA

	Measured	Allowed
Outside Tube Diameter - Dt (inches)	0.250	NA
Base To Opening Distance - Pa (inches)	0.36	NA
Base To Opening Distance - Pb (inches)	0.369	NA
Pa/Dt	1.44	1.05-1.50
Pb/Dt	1.48	1.05-1.50
Angle $\alpha 1$ ($^{\circ}$)	2.2	10
Angle $\alpha 2$ ($^{\circ}$)	2.4	10
Angle B1($^{\circ}$)	4	5
Angle B1($^{\circ}$)	2.6	5
Opening to Opening Distance Pa+Pb (inches)	0.729	NA
Angle Z ($^{\circ}$)	0.6	NA
z (inches)	0.0076	0.125
Angle W ($^{\circ}$)	0.4	NA
w (inches)	0.005	0.031

Note Any Damage, Nicks or Dents to the Pitot Tube

Is the Pitot Tube Part of an Assembly Yes
If Yes, Complete the Section Below

Pitot	Measured	Minimum
Distance From Nozzle (inches)	0.75	0.75 in.
Pitot to Thermocouple Distance (inches)	2	2 in.
Pitot to Sample Probe Distance (inches)	4.75	3 in.

Does the Pitot Tube Meet the Above Requirements Yes
Is the Pitot Tube Free of Damage Yes

If Yes to Both, a Pitot Tube Coefficient of 0.84 is Assigned
If No to Either, then the Pitot Tube Must be Calibrated

Airtech Environmental Services, Inc.
S-Type Pitot Tube Inspection Form

Date January 17, 2011
 Pitot ID AE5-10-1
 Operator A. Kienitz

	Measured	Allowed
Outside Tube Diameter - Dt (inches)	0.250	NA
Base To Opening Distance - Pa (inches)	0.363	NA
Base To Opening Distance - Pb (inches)	0.359	NA
Pa/Dt	1.452	1.05-1.50
Pb/Dt	1.436	1.05-1.50
Angle, $\alpha 1(^{\circ})$	2	10
Angle, $\alpha 2(^{\circ})$	2	10
Angle, B1($^{\circ}$)	2	5
Angle, B1($^{\circ}$)	4	5
Opening to Opening Distance Pa+Pb (inches)	0.722	NA
Angle, Z ($^{\circ}$)	89	NA
z (inches)	0.015	0.125
Angle, W ($^{\circ}$)	91	NA
w (inches)	0.010	0.031
Pitot to Thermocouple Distance, W (inches)	2.125	≥ 2

Note Any Damage, Nicks or Dents to the Pitot Tube

Is the Pitot Tube Part of an Assembly **Yes**
 If Yes, Complete the Section Below

Pitot	Measured	Minimum
Distance From Nozzle, X (inches)	0.75	0.75
Pitot to Sample Probe Distance, Y (inches)	4.25	3

Does the Pitot Tube Meet the Above Requirements **Yes**
 Is the Pitot Tube Free of Damage **Yes**

If Yes to Both, a Pitot Tube Coefficient of 0.84 is Assigned
 If No to Either, then the Pitot Tube Must be Calibrated

Airtech Environmental Services, Inc.
S-Type Pitot Tube Inspection Form

Date 1/26/11
Pitot ID AE5-10-2
Operator EA

	Measured	Allowed
Outside Tube Diameter - Dt (inches)	0.250	NA
Base To Opening Distance - Pa (inches)	0.346	NA
Base To Opening Distance - Pb (inches)	0.346	NA
Pa/Dt	1.38	1.05-1.50
Pb/Dt	1.38	1.05-1.50
Angle $\alpha 1(^{\circ})$	1.3	10
Angle $\alpha 2(^{\circ})$	1.6	10
Angle B1($^{\circ}$)	4.3	5
Angle B1($^{\circ}$)	2.3	5
Opening to Opening Distance Pa+Pb (inches)	0.704	NA
Angle Z ($^{\circ}$)	3.9	NA
z (inches)	0.0479	0.125
Angle W ($^{\circ}$)	0.7	NA
w (inches)	0.009	0.031

Note Any Damage, Nicks or Dents to the Pitot Tube

Is the Pitot Tube Part of an Assembly Yes
If Yes, Complete the Section Below

Pitot	Measured	Minimum
Distance From Nozzle (inches)	0.75	0.75 in.
Pitot to Thermocouple Distance (inches)	3	2 in.
Pitot to Sample Probe Distance (inches)	5.5	3 in.

Does the Pitot Tube Meet the Above Requirements Yes
Is the Pitot Tube Free of Damage Yes

If Yes to Both, a Pitot Tube Coefficient of 0.84 is Assigned
If No to Either, then the Pitot Tube Must be Calibrated

Airtech Environmental Services, Inc.
S-Type Pitot Tube Inspection Form

Date 1/26/11
Pitot ID AE-5-10-3
Operator EA

	Measured	Allowed
Outside Tube Diameter - Dt (inches)	0.250	NA
Base To Opening Distance - Pa (inches)	0.357	NA
Base To Opening Distance - Pb (inches)	0.357	NA
Pa/Dt	1.43	1.05-1.50
Pb/Dt	1.43	1.05-1.50
Angle $\alpha 1$ (°)	2	10
Angle $\alpha 2$ (°)	0.8	10
Angle B1 (°)	2.5	5
Angle B1 (°)	3.9	5
Opening to Opening Distance Pa+Pb (inches)	0.714	NA
Angle Z (°)	2.5	NA
z (inches)	0.0311	0.125
Angle W (°)	0.2	NA
w (inches)	0.002	0.031

Note Any Damage, Nicks or Dents to the Pitot Tube

Is the Pitot Tube Part of an Assembly Yes
If Yes, Complete the Section Below

Pitot	Measured	Minimum
Distance From Nozzle (inches)	0.75	0.75 in.
Pitot to Thermocouple Distance (inches)	2.5	2 in.
Pitot to Sample Probe Distance (inches)	4.25	3 in.

Does the Pitot Tube Meet the Above Requirements Yes
Is the Pitot Tube Free of Damage Yes

If Yes to Both, a Pitot Tube Coefficient of 0.84 is Assigned
If No to Either, then the Pitot Tube Must be Calibrated

Airtech Environmental Services, Inc.
S-Type Pitot Tube Inspection Form

Date January 19, 2011
Pitot ID AE5-12-1
Operator A. Kienitz

	Measured	Allowed
Outside Tube Diameter - Dt (inches)	0.250	NA
Base To Opening Distance - Pa (inches)	0.312	NA
Base To Opening Distance - Pb (inches)	0.333	NA
Pa/Dt	1.248	1.05-1.50
Pb/Dt	1.332	1.05-1.50
Angle, $\alpha 1(^{\circ})$	1	10
Angle, $\alpha 2(^{\circ})$	0	10
Angle, B1($^{\circ}$)	2	5
Angle, B1($^{\circ}$)	3	5
Opening to Opening Distance Pa+Pb (inches)	0.645	NA
Angle, Z ($^{\circ}$)	89	NA
z (inches)	0.041	0.125
Angle, W ($^{\circ}$)	90	NA
w (inches)	0.011	0.031
Pitot to Thermocouple Distance, W (inches)	2.00	≥ 2

Note Any Damage, Nicks or Dents to the Pitot Tube

Is the Pitot Tube Part of an Assembly **YES**

If Yes, Complete the Section Below

Pitot	Measured	Minimum
Distance From Nozzle, X (inches)	0.75	0.75
Pitot to Sample Probe Distance, Y (inches)	4.75	3

Does the Pitot Tube Meet the Above Requirements **Yes**

Is the Pitot Tube Free of Damage **Yes**

If Yes to Both, a Pitot Tube Coefficient of 0.84 is Assigned

If No to Either, then the Pitot Tube Must be Calibrated

Airtech Environmental Services, Inc.
S-Type Pitot Tube Inspection Form

Date 1/26/11
Pitot ID AE5-12-2
Operator EA

	Measured	Allowed
Outside Tube Diameter - Dt (inches)	0.250	NA
Base To Opening Distance - Pa (inches)	0.34	NA
Base To Opening Distance - Pb (inches)	0.34	NA
Pa/Dt	1.36	1.05-1.50
Pb/Dt	1.36	1.05-1.50
Angle $\alpha 1(^{\circ})$	0.4	10
Angle $\alpha 2(^{\circ})$	1	10
Angle B1($^{\circ}$)	0.9	5
Angle B1($^{\circ}$)	0.1	5
Opening to Opening Distance Pa+Pb (inches)	0.680	NA
Angle Z ($^{\circ}$)	3.2	NA
z (inches)	0.0380	0.125
Angle W ($^{\circ}$)	0.2	NA
w (inches)	0.002	0.031

Note Any Damage, Nicks or Dents to the Pitot Tube

Is the Pitot Tube Part of an Assembly Yes
If Yes, Complete the Section Below

Pitot	Measured	Minimum
Distance From Nozzle (inches)	0.75	0.75 in.
Pitot to Thermocouple Distance (inches)	2.25	2 in.
Pitot to Sample Probe Distance (inches)	6	3 in.

Does the Pitot Tube Meet the Above Requirements Yes
Is the Pitot Tube Free of Damage Yes

If Yes to Both, a Pitot Tube Coefficient of 0.84 is Assigned
If No to Either, then the Pitot Tube Must be Calibrated

Airtech Environmental Services, Inc.
S-Type Pitot Tube Inspection Form

Date January 26, 2011
 Pitot ID AE5-12-3
 Operator EA

	Measured	Allowed
Outside Tube Diameter - Dt (inches)	0.250	NA
Base To Opening Distance - Pa (inches)	0.338	NA
Base To Opening Distance - Pb (inches)	0.338	NA
Pa/Dt	1.35	1.05-1.50
Pb/Dt	1.35	1.05-1.50
Angle $\alpha 1(^{\circ})$	1.1	10
Angle $\alpha 2(^{\circ})$	1.1	10
Angle B1($^{\circ}$)	2.1	5
Angle B2($^{\circ}$)	3.5	5
Opening to Opening Distance Pa+Pb (inches)	0.676	NA
Angle Z ($^{\circ}$)	4.3	NA
z (inches)	0.05	0.125
Angle W ($^{\circ}$)	0.9	NA
w (inches)	0.01	0.031

Note Any Damage, Nicks or Dents to the Pitot Tube

Is the Pitot Tube Part of an Assembly Yes
 If Yes, Complete the Section Below

	Measured	Allowed
Distance From Nozzle, X (inches)	0.75	0.75 in.
Pitot to Thermocouple Distance, W (inches)	2.25	2 in.
Pitot to Sample Probe Distance, Y (inches)	3.500	3 in.

Does the Pitot Tube Meet the Above Requirements Yes
 Is the Pitot Tube Free of Damage Yes

If Yes to Both, a Pitot Tube Coefficient of 0.84 is Assigned
 If No to Either, then the Pitot Tube Must be Calibrated